

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
 Data File : VV035170.D
 Acq On : 12 Apr 2024 13:53
 Operator : SY/MD
 Sample : P2056-05DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	66670	71102	10.50%	1.337%
2	1.532	145	153	167	rVB	71420	85331	12.60%	1.605%
3	2.056	306	316	333	rVB	125098	181542	26.80%	3.414%
4	2.445	427	437	451	rBV2	6454	11907	1.76%	0.224%
5	2.555	460	471	473	rBV2	5506	7814	1.15%	0.147%
6	3.841	851	871	912	rBV2	50018	296587	43.78%	5.577%
7	4.249	982	998	1022	rBV2	88616	236202	34.87%	4.441%
8	4.957	1205	1218	1256	rBV2	207675	538193	79.45%	10.120%
9	5.535	1387	1398	1429	rBV	179215	397929	58.74%	7.482%
10	5.989	1527	1539	1562	rBV	122569	263464	38.89%	4.954%
11	6.918	1819	1828	1851	rBV	42164	88304	13.04%	1.660%
12	7.243	1918	1929	1954	rBV	203238	384283	56.73%	7.226%
13	7.564	2019	2029	2052	rBV3	23790	55123	8.14%	1.036%
14	7.902	2114	2134	2161	rBV	388374	677386	100.00%	12.737%
15	8.030	2165	2174	2210	rBV	237311	559625	82.62%	10.523%
16	8.786	2397	2409	2431	rBV	295607	503979	74.40%	9.476%
17	10.153	2824	2834	2852	rBV	95264	156477	23.10%	2.942%
18	10.326	2878	2888	2900	rVB2	8796	15671	2.31%	0.295%
19	11.185	3145	3155	3181	rBV	268549	441645	65.20%	8.304%
20	11.561	3259	3272	3293	rBV	212692	345637	51.03%	6.499%




Sum of corrected areas: 5318201

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035170.D
Acq On : 12 Apr 2024 13:53
Operator : SY/MD
Sample : P2056-05DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

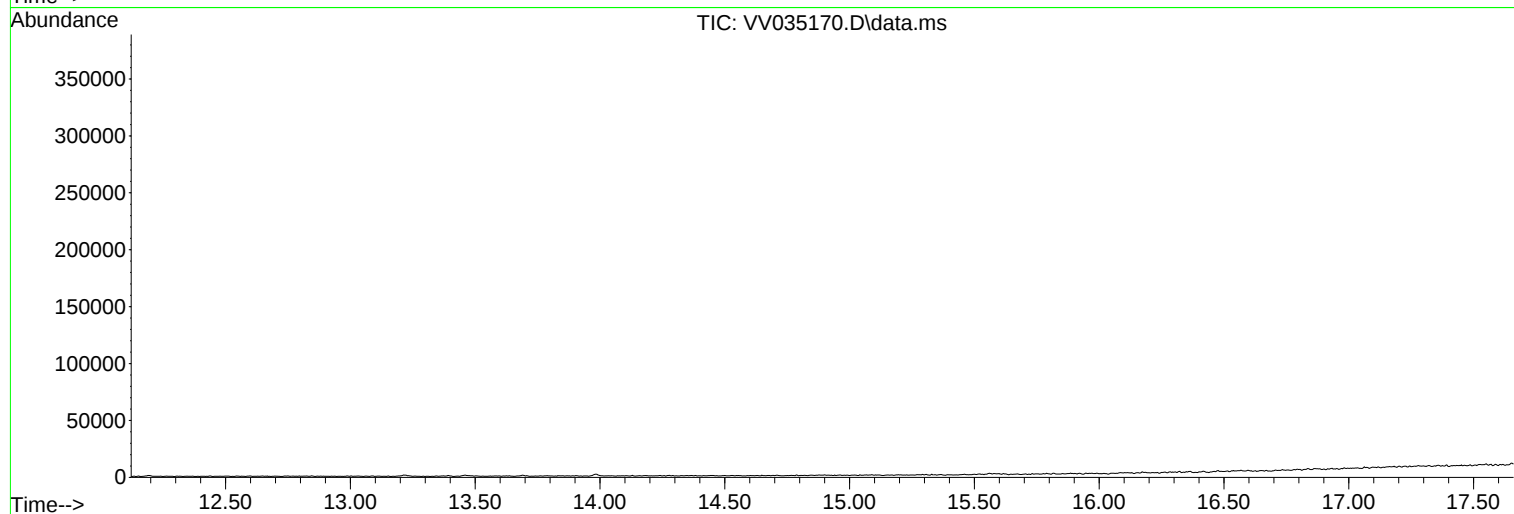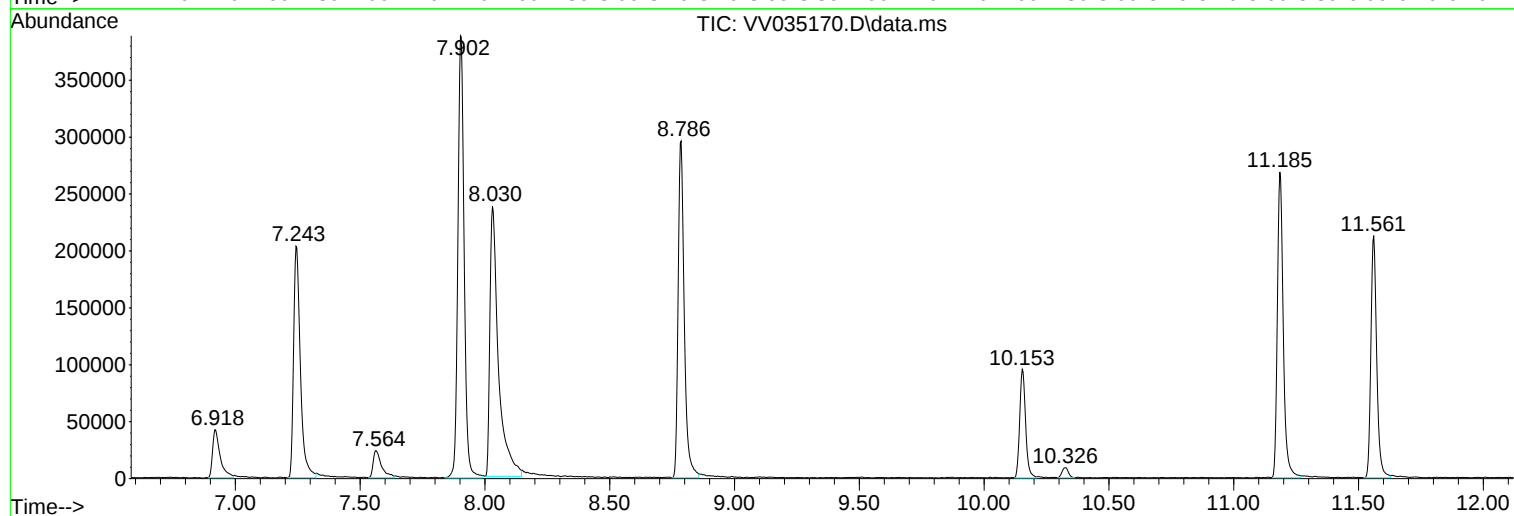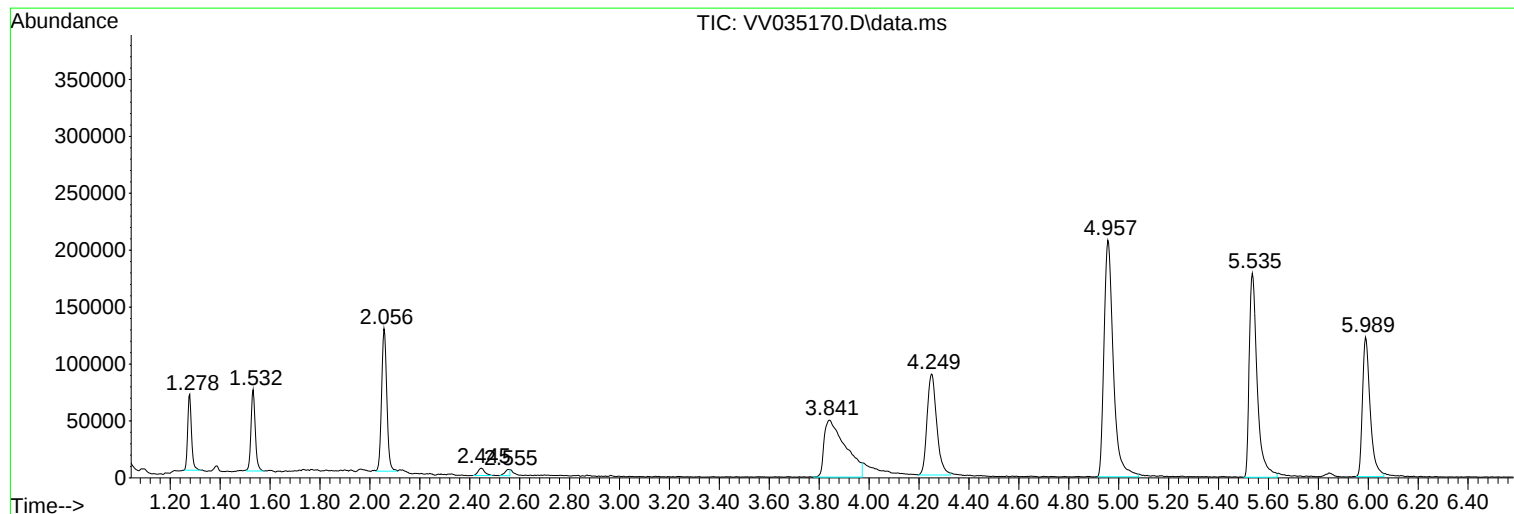

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035170.D
Acq On : 12 Apr 2024 13:53
Operator : SY/MD
Sample : P2056-05DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035170.D
Acq On : 12 Apr 2024 13:53
Operator : SY/MD
Sample : P2056-05DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------