

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
 Data File : VV035171.D
 Acq On : 12 Apr 2024 14:17
 Operator : SY/MD
 Sample : P2056-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035171.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	88	rVB	72387	78594	14.55%	1.622%
2	1.385	100	107	115	rVB	28568	33002	6.11%	0.681%
3	1.529	145	152	174	rVB	73004	89311	16.53%	1.843%
4	1.963	282	287	297	rVB2	5623	8258	1.53%	0.170%
5	2.057	305	316	330	rBV	123385	180738	33.46%	3.729%
6	3.847	850	873	924	rBV3	67668	398573	73.79%	8.224%
7	4.249	985	998	1024	rVB2	89691	238021	44.07%	4.911%
8	4.957	1204	1218	1253	rBV2	201435	520113	96.29%	10.732%
9	5.535	1385	1398	1427	rBV	193866	423993	78.50%	8.749%
10	5.989	1526	1539	1569	rBV2	118047	263405	48.77%	5.435%
11	6.921	1814	1829	1853	rBV	39583	86230	15.96%	1.779%
12	7.246	1917	1930	1952	rBV	198893	374620	69.35%	7.730%
13	7.564	2020	2029	2048	rBV2	22600	48632	9.00%	1.003%
14	7.876	2113	2126	2131	rBV	13608	23165	4.29%	0.478%
15	7.912	2132	2137	2151	rVB5	10992	18955	3.51%	0.391%
16	8.031	2161	2174	2228	rBV	185414	532230	98.53%	10.982%
17	8.786	2396	2409	2435	rBV	307355	540150	100.00%	11.146%
18	10.153	2824	2834	2855	rBV	89111	150519	27.87%	3.106%
19	10.323	2878	2887	2898	rVB	29607	47516	8.80%	0.980%
20	11.185	3144	3155	3180	rBV	283876	458107	84.81%	9.453%
21	11.561	3259	3272	3294	rBV	196845	332214	61.50%	6.855%




Sum of corrected areas: 4846346

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035171.D
Acq On : 12 Apr 2024 14:17
Operator : SY/MD
Sample : P2056-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

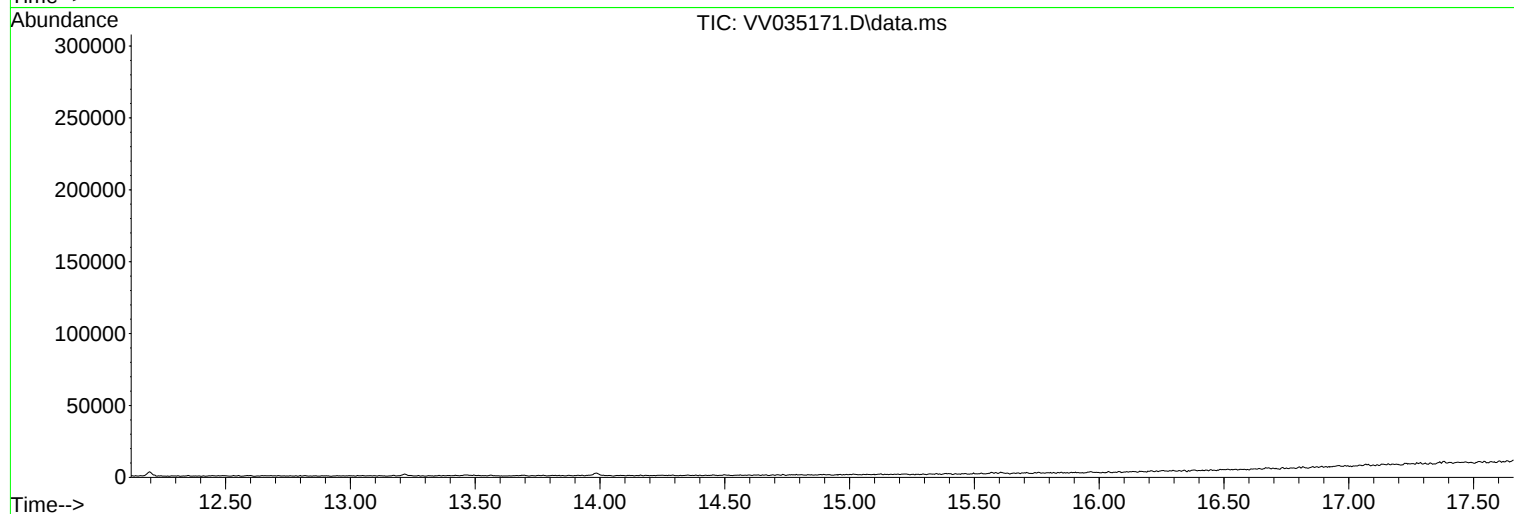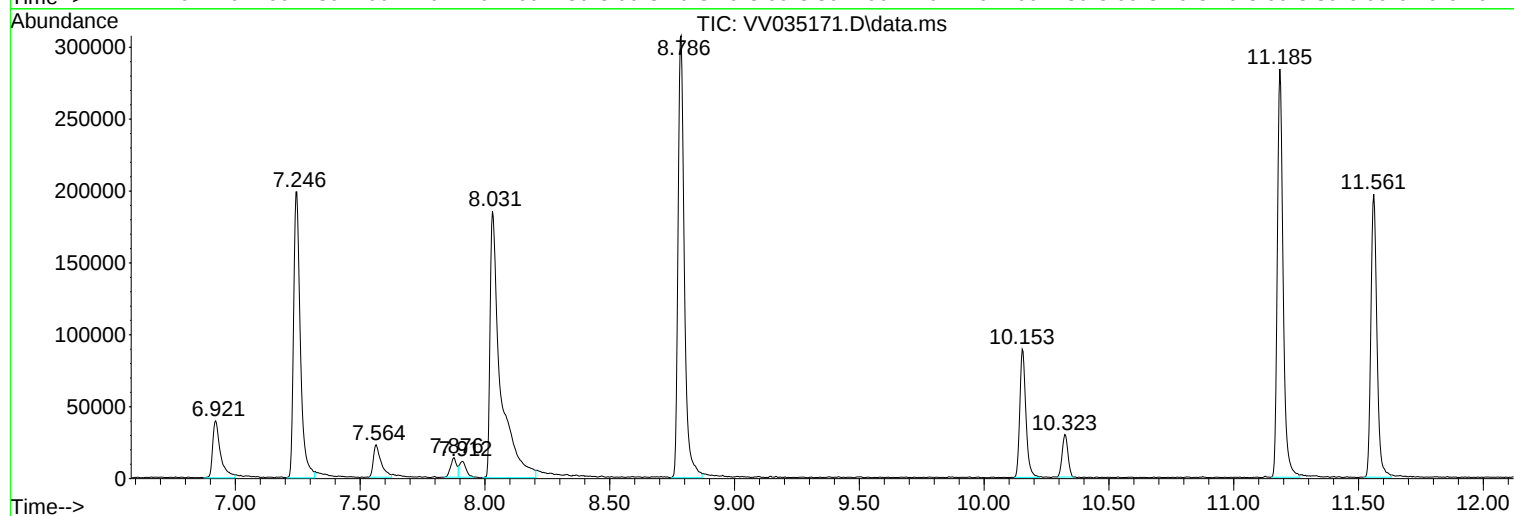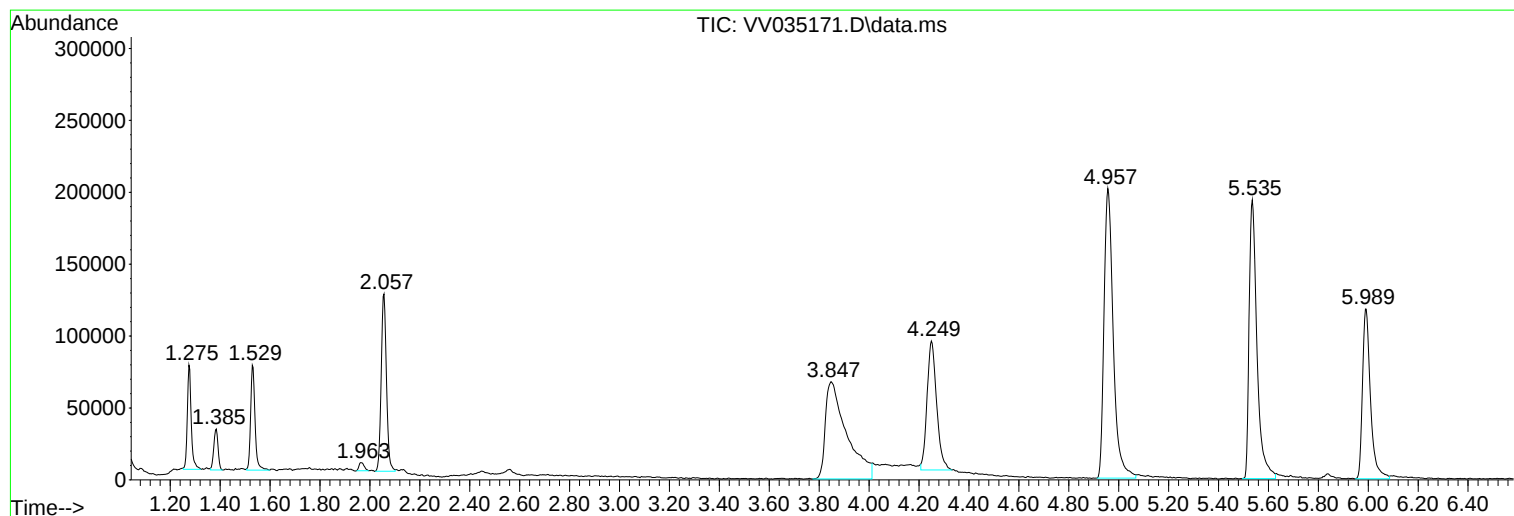

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035171.D
Acq On : 12 Apr 2024 14:17
Operator : SY/MD
Sample : P2056-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035171.D
Acq On : 12 Apr 2024 14:17
Operator : SY/MD
Sample : P2056-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc