

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
 Data File : VV035174.D
 Acq On : 12 Apr 2024 15:28
 Operator : SY/MD
 Sample : P2056-09DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BQ9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035174.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVB	69613	76167	13.78%	1.479%
2	1.384	101	107	116	rVB	15005	17504	3.17%	0.340%
3	1.532	146	153	166	rVB	74450	88026	15.92%	1.709%
4	2.060	306	317	329	rBV	114316	169124	30.59%	3.284%
5	2.452	429	439	451	rVB4	5991	10805	1.95%	0.210%
6	3.815	846	863	896	rBV4	54868	232873	42.12%	4.522%
7	4.249	984	998	1029	rVB	92544	246779	44.63%	4.792%
8	4.960	1202	1219	1250	rBV2	204595	540798	97.81%	10.500%
9	5.535	1387	1398	1432	rBV	192811	426265	77.09%	8.277%
10	5.992	1527	1540	1565	rBV	123609	271762	49.15%	5.277%
11	6.921	1819	1829	1859	rBV2	40304	89878	16.26%	1.745%
12	7.246	1919	1930	1967	rBV	206911	388158	70.20%	7.537%
13	7.564	2018	2029	2047	rBV2	23786	49254	8.91%	0.956%
14	7.905	2118	2135	2156	rBV	251030	441376	79.83%	8.570%
15	8.030	2165	2174	2223	rBV	201824	552918	100.00%	10.736%
16	8.786	2392	2409	2442	rBV	315206	548833	99.26%	10.656%
17	10.153	2821	2834	2857	rBV	94885	161952	29.29%	3.145%
18	10.323	2875	2887	2902	rVB2	9037	15978	2.89%	0.310%
19	11.185	3144	3155	3182	rBV	289772	472146	85.39%	9.167%
20	11.561	3261	3272	3289	rBV	213729	349623	63.23%	6.789%




Sum of corrected areas: 5150219

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035174.D
Acq On : 12 Apr 2024 15:28
Operator : SY/MD
Sample : P2056-09DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

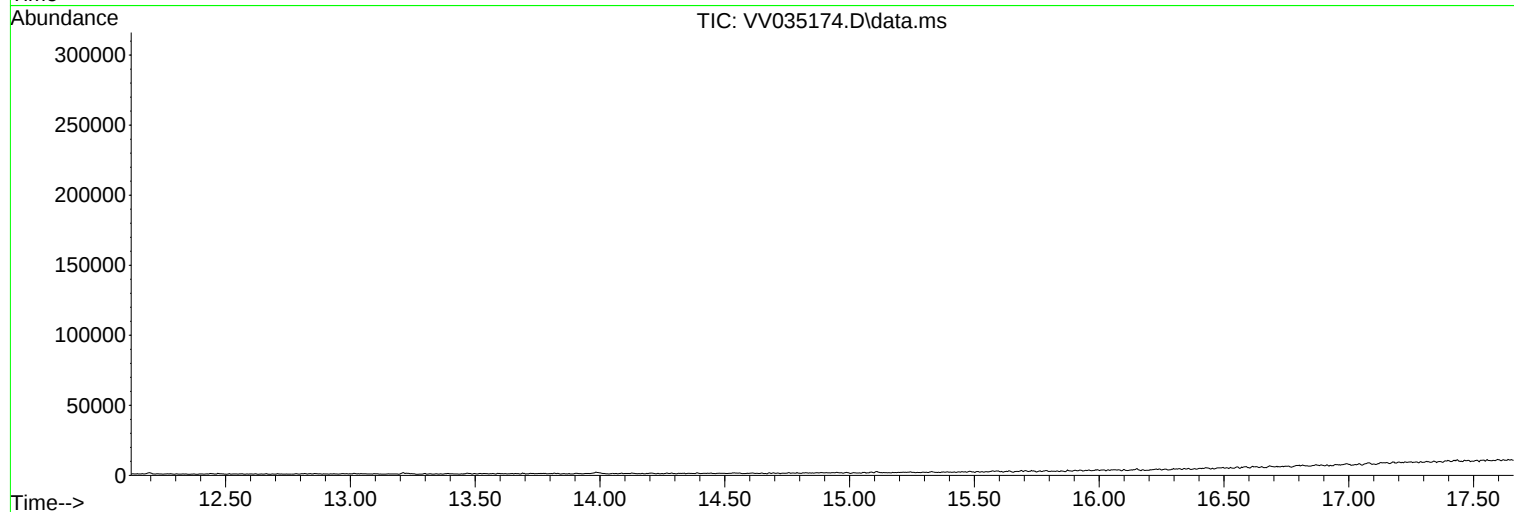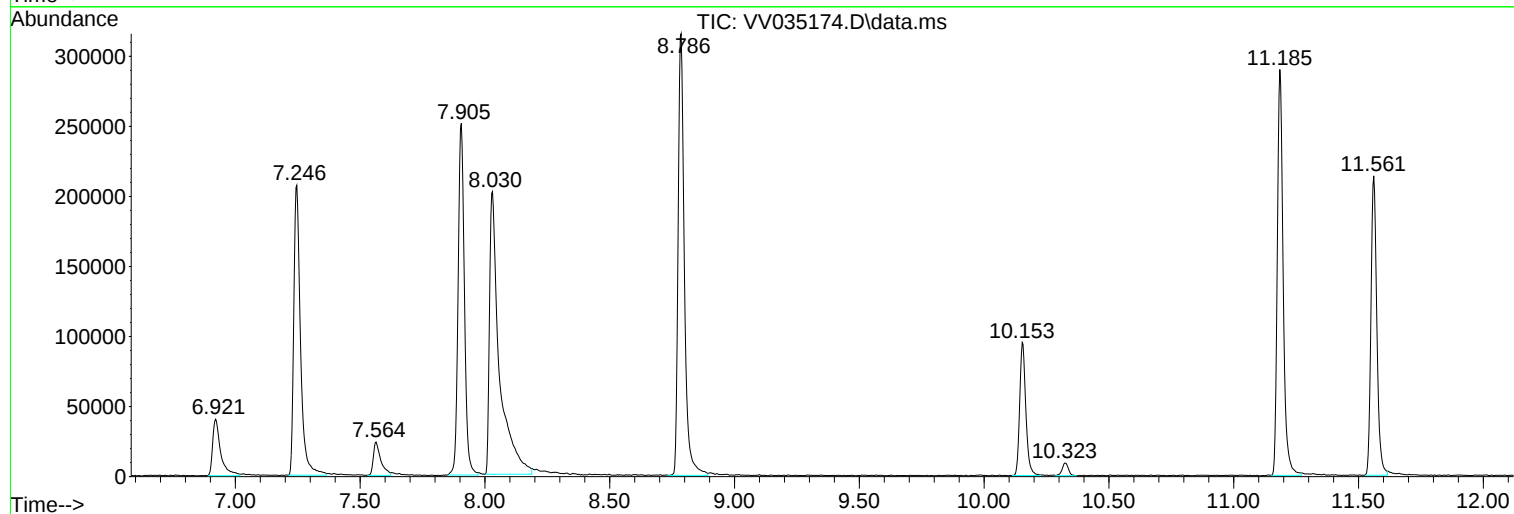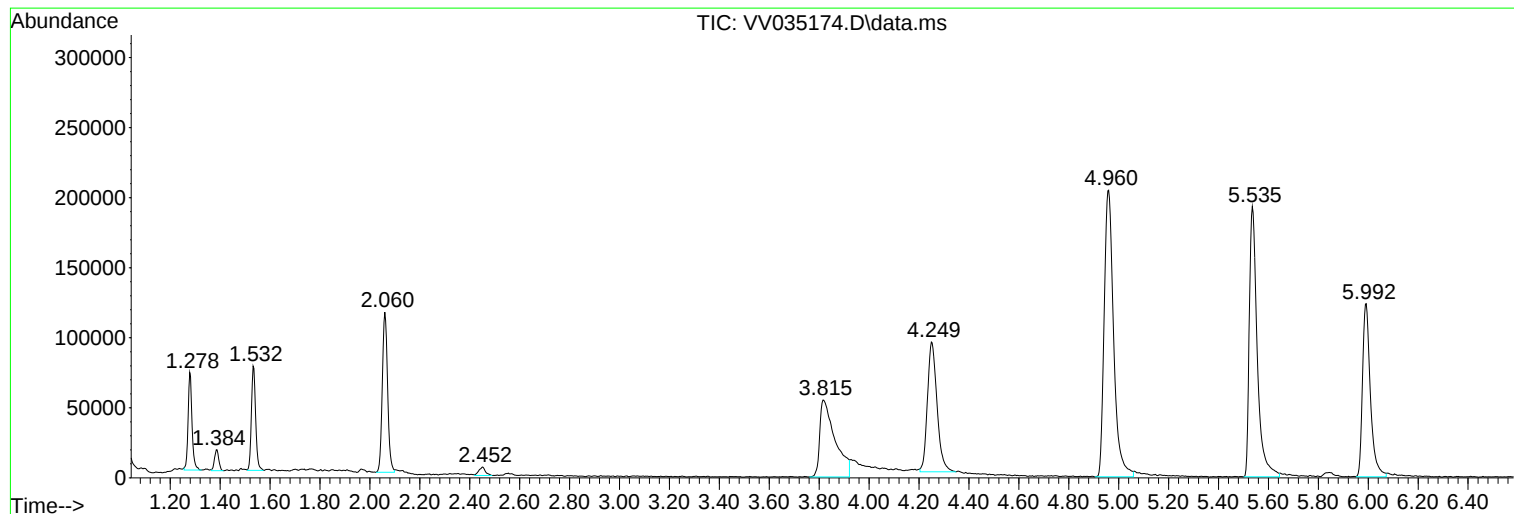

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035174.D
Acq On : 12 Apr 2024 15:28
Operator : SY/MD
Sample : P2056-09DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035174.D
Acq On : 12 Apr 2024 15:28
Operator : SY/MD
Sample : P2056-09DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BQ9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc