

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
 Data File : VV035175.D
 Acq On : 12 Apr 2024 15:52
 Operator : SY/MD
 Sample : P2056-10DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BS4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035175.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	85	rVB	66357	69577	13.10%	1.419%
2	1.384	101	107	114	rVB	14220	16256	3.06%	0.332%
3	1.532	145	153	168	rVB	72882	86281	16.24%	1.760%
4	2.056	306	316	330	rBV	115189	166584	31.36%	3.398%
5	2.445	428	437	449	rBV2	5613	10124	1.91%	0.207%
6	3.841	855	871	903	rBV4	48638	235588	44.36%	4.805%
7	4.249	981	998	1024	rVB2	88885	234666	44.18%	4.787%
8	4.957	1202	1218	1252	rBV3	199183	516653	97.27%	10.538%
9	5.535	1387	1398	1425	rBV	177306	384770	72.44%	7.848%
10	5.850	1482	1496	1500	rBV	2594	5457	1.03%	0.111%
11	5.989	1527	1539	1565	rBV	119093	258694	48.71%	5.277%
12	6.921	1817	1829	1855	rBV2	38783	86337	16.26%	1.761%
13	7.246	1919	1930	1954	rBV	190502	360513	67.88%	7.353%
14	7.564	2016	2029	2054	rBV	21800	49250	9.27%	1.005%
15	7.905	2113	2135	2162	rBV	258730	464621	87.48%	9.477%
16	8.030	2162	2174	2221	rBV	198876	531141	100.00%	10.834%
17	8.786	2398	2409	2435	rBV	291358	499052	93.96%	10.179%
18	10.152	2823	2834	2852	rBV	91886	153660	28.93%	3.134%
19	10.323	2877	2887	2897	rVB	8627	14308	2.69%	0.292%
20	11.185	3144	3155	3180	rBV	263498	429012	80.77%	8.751%
21	11.561	3260	3272	3294	rBV	197787	330093	62.15%	6.733%




Sum of corrected areas: 4902637

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035175.D
Acq On : 12 Apr 2024 15:52
Operator : SY/MD
Sample : P2056-10DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BS4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

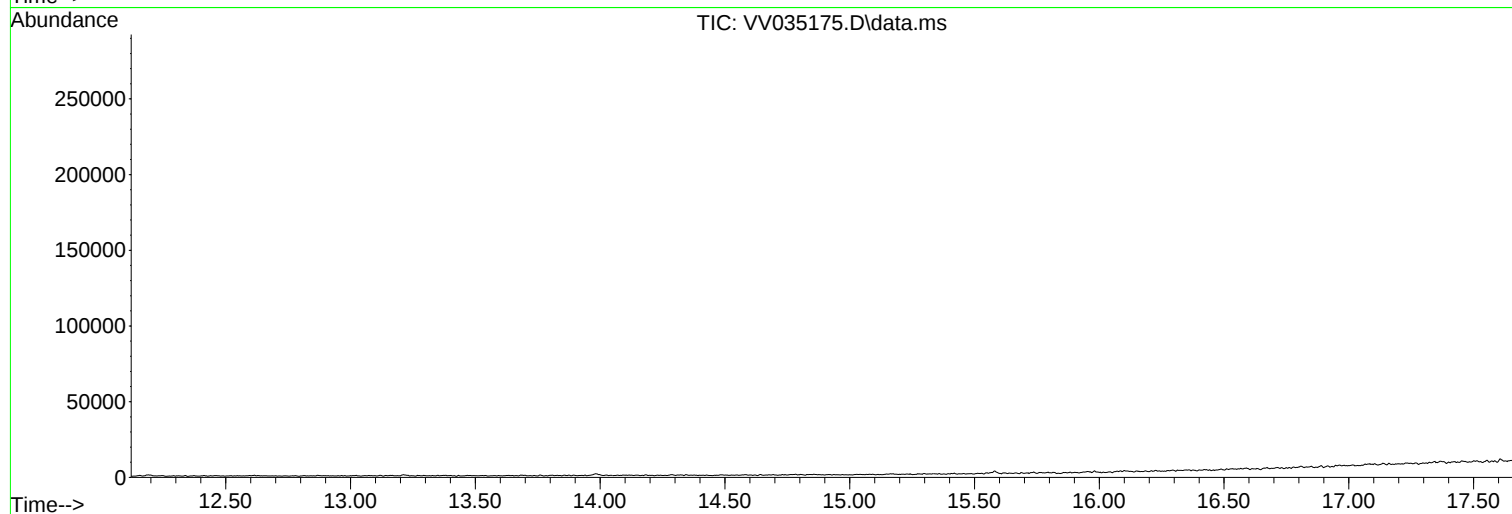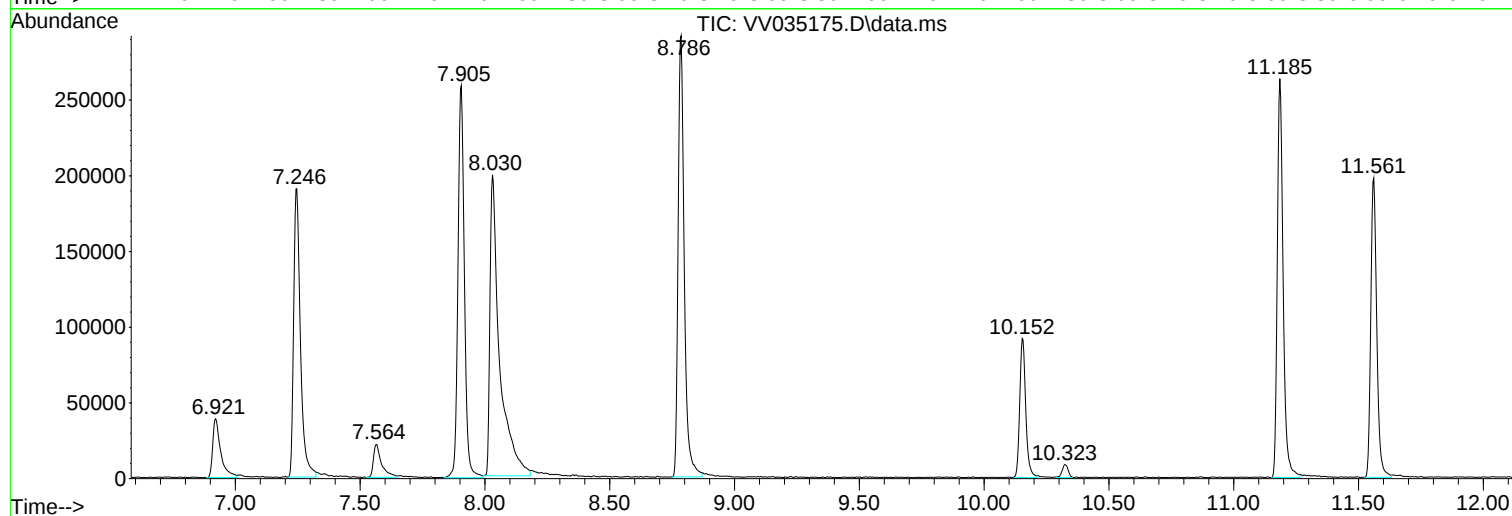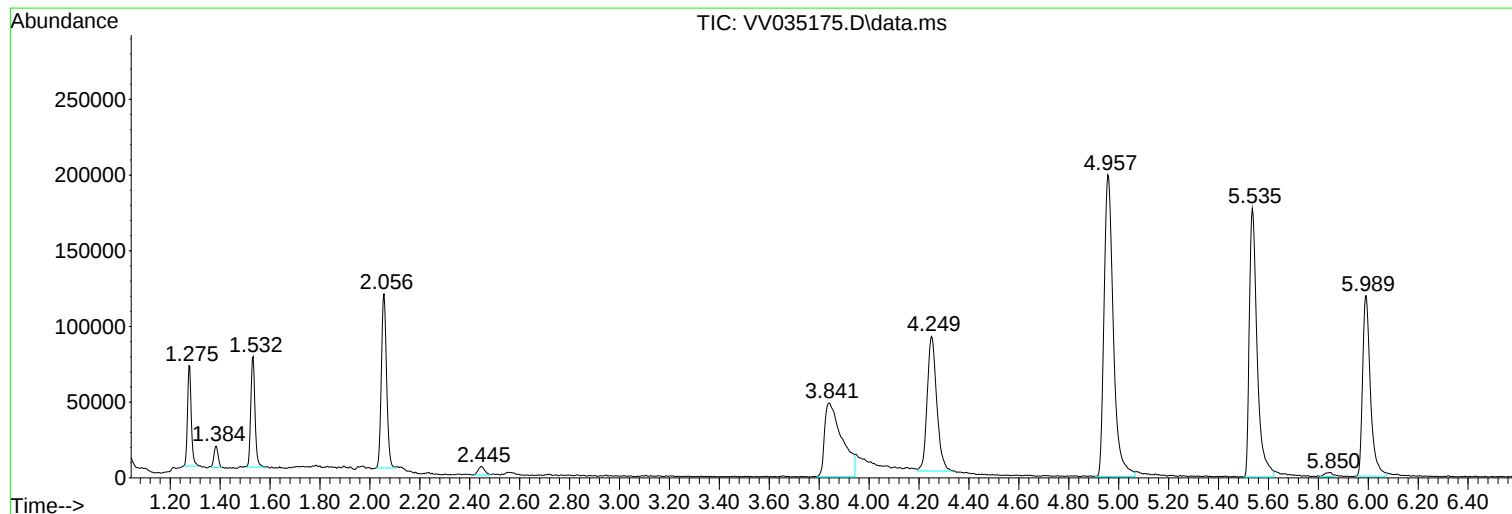

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035175.D
Acq On : 12 Apr 2024 15:52
Operator : SY/MD
Sample : P2056-10DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BS4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035175.D
Acq On : 12 Apr 2024 15:52
Operator : SY/MD
Sample : P2056-10DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BS4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc