

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
 Data File : VV035182.D
 Acq On : 12 Apr 2024 18:39
 Operator : SY/MD
 Sample : P2057-07DL 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BL8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035182.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rVB	60288	63640	10.24%	1.432%
2	1.532	146	153	165	rBV	62840	73268	11.79%	1.649%
3	2.060	307	317	334	rVB	111743	170051	27.37%	3.827%
4	2.449	428	438	450	rVB5	4657	8897	1.43%	0.200%
5	2.558	463	472	484	rBV2	3519	6547	1.05%	0.147%
6	3.828	847	867	910	rBV3	56886	307444	49.48%	6.919%
7	4.249	984	998	1025	rBV	79542	211088	33.97%	4.751%
8	4.957	1203	1218	1246	rBV2	186690	483756	77.85%	10.887%
9	5.535	1387	1398	1435	rBV	151589	332673	53.54%	7.487%
10	5.989	1522	1539	1566	rBV	112041	247461	39.82%	5.569%
11	6.921	1819	1829	1852	rBV	37715	80753	13.00%	1.817%
12	7.246	1919	1930	1962	rBV	174223	328322	52.84%	7.389%
13	7.561	2019	2028	2053	rBV2	21597	46921	7.55%	1.056%
14	7.905	2115	2135	2155	rBV3	97209	180419	29.03%	4.060%
15	8.031	2164	2174	2218	rBV	271940	621400	100.00%	13.985%
16	8.786	2398	2409	2436	rBV	244193	426263	68.60%	9.593%
17	10.153	2823	2834	2851	rBV	104536	167755	27.00%	3.775%
18	10.323	2877	2887	2901	rVB2	8662	12977	2.09%	0.292%
19	11.185	3144	3155	3178	rBV	221679	364090	58.59%	8.194%
20	11.561	3258	3272	3293	rBV	183878	309625	49.83%	6.968%




Sum of corrected areas: 4443350

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035182.D
Acq On : 12 Apr 2024 18:39
Operator : SY/MD
Sample : P2057-07DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BL8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

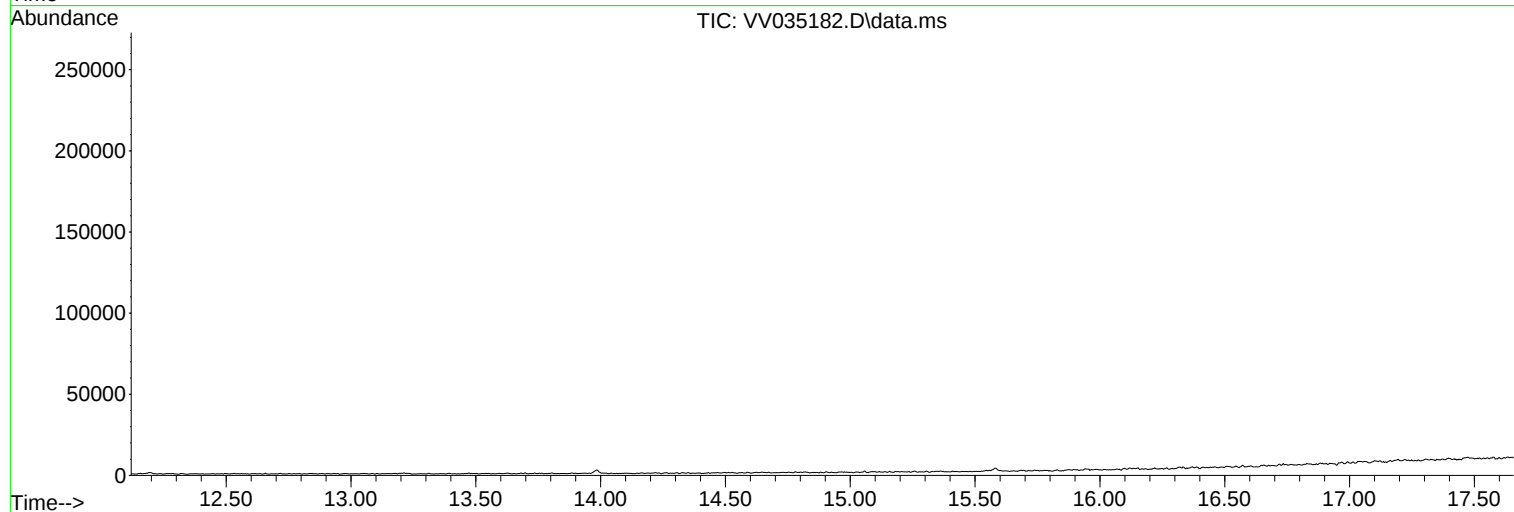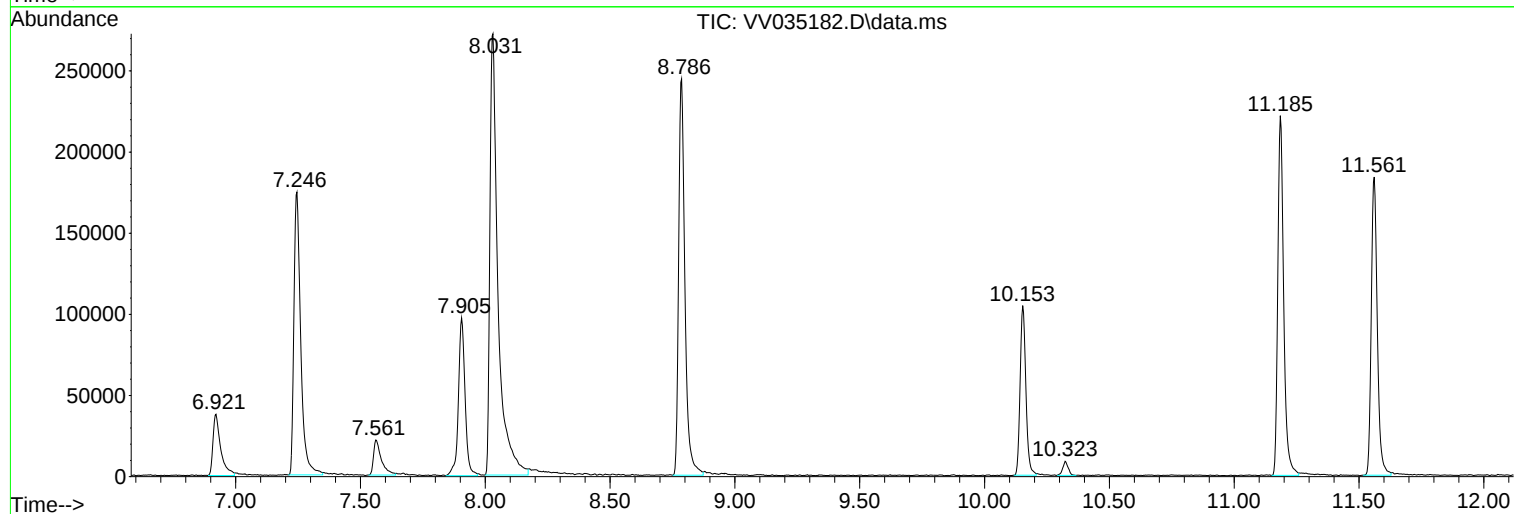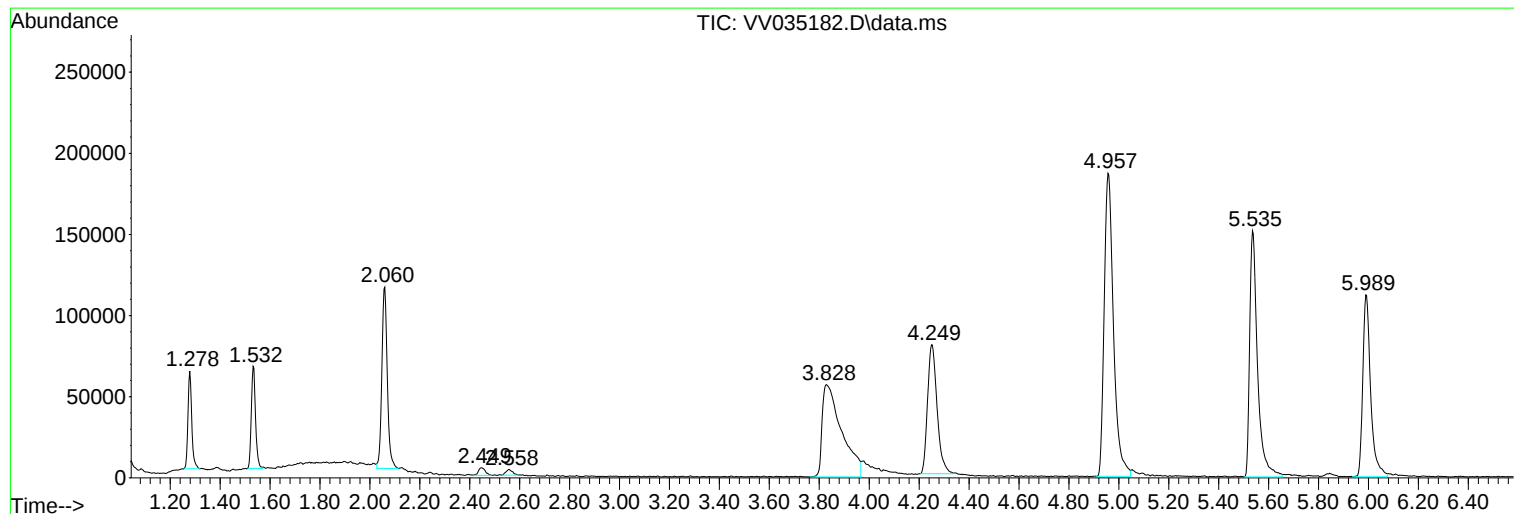

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035182.D
Acq On : 12 Apr 2024 18:39
Operator : SY/MD
Sample : P2057-07DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BL8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035182.D
Acq On : 12 Apr 2024 18:39
Operator : SY/MD
Sample : P2057-07DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BL8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------