

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
 Data File : VV035183.D
 Acq On : 12 Apr 2024 19:03
 Operator : SY/MD
 Sample : P2057-10DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BM8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV035183.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	66952	70332	12.10%	1.418%
2	1.532	146	153	168	rVB	72689	86105	14.81%	1.736%
3	2.060	307	317	335	rVB	121767	179773	30.92%	3.624%
4	2.452	429	439	446	rBV4	5324	9277	1.60%	0.187%
5	3.818	849	864	901	rBV2	48972	225365	38.76%	4.543%
6	4.249	983	998	1029	rVB	92768	246271	42.36%	4.964%
7	4.957	1203	1218	1255	rBV3	208421	549123	94.44%	11.069%
8	5.535	1388	1398	1429	rBV	175110	381940	65.69%	7.699%
9	5.989	1527	1539	1566	rBV	126750	277486	47.72%	5.593%
10	6.921	1818	1829	1861	rBV	41479	91229	15.69%	1.839%
11	7.246	1919	1930	1955	rBV	205934	388181	66.76%	7.825%
12	7.564	2018	2029	2051	rBV	23280	50636	8.71%	1.021%
13	7.905	2114	2135	2162	rBV	202151	358736	61.70%	7.231%
14	8.030	2165	2174	2219	rBV	213245	581438	100.00%	11.720%
15	8.786	2397	2409	2439	rBV	288915	499424	85.89%	10.067%
16	10.152	2823	2834	2857	rBV	100972	169987	29.24%	3.426%
17	10.326	2880	2888	2898	rVB2	5436	8174	1.41%	0.165%
18	11.185	3144	3155	3176	rBV	263099	426727	73.39%	8.602%
19	11.561	3260	3272	3299	rBV	219793	360820	62.06%	7.273%




Sum of corrected areas: 4961024

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035183.D
Acq On : 12 Apr 2024 19:03
Operator : SY/MD
Sample : P2057-10DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BM8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

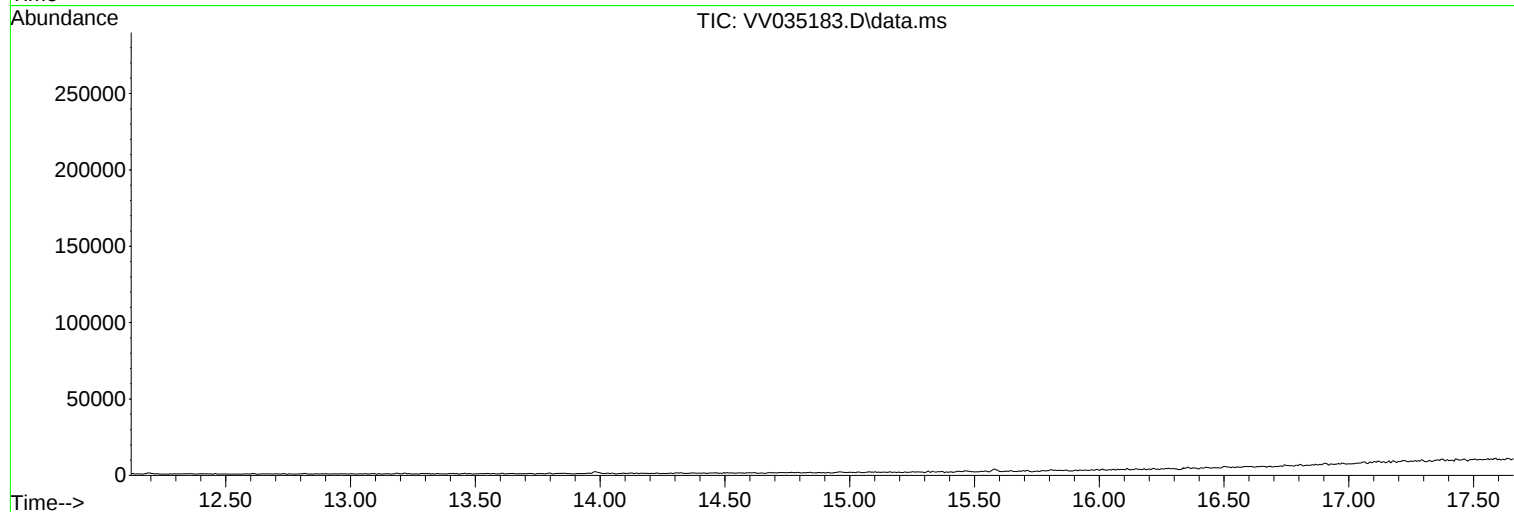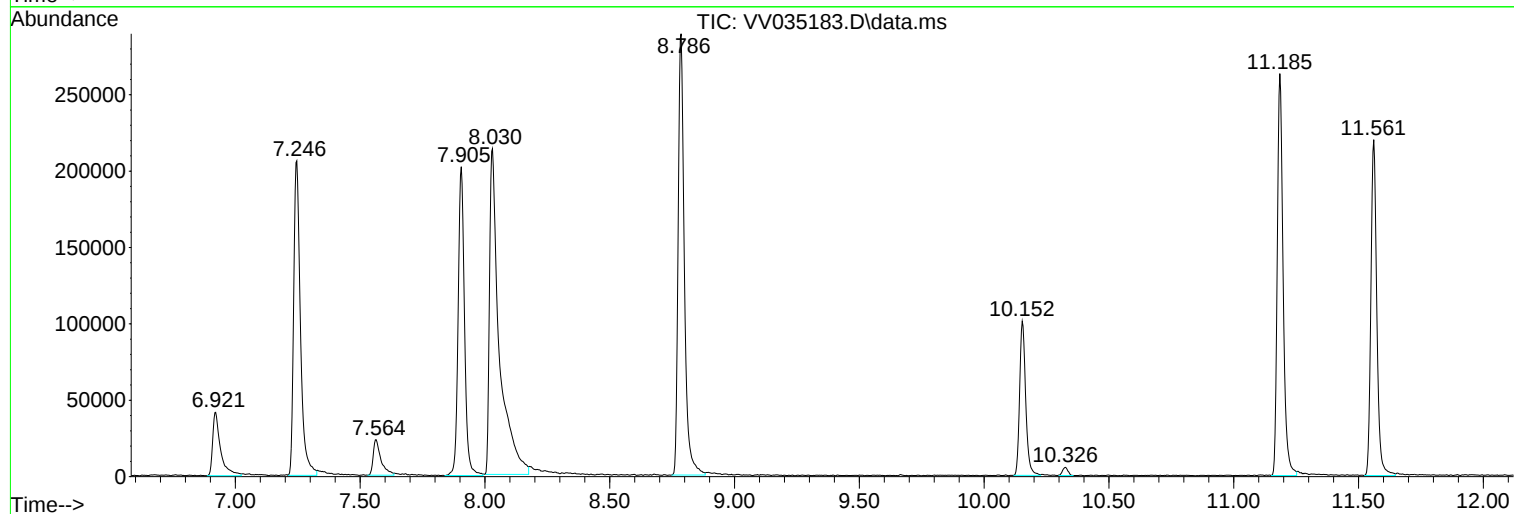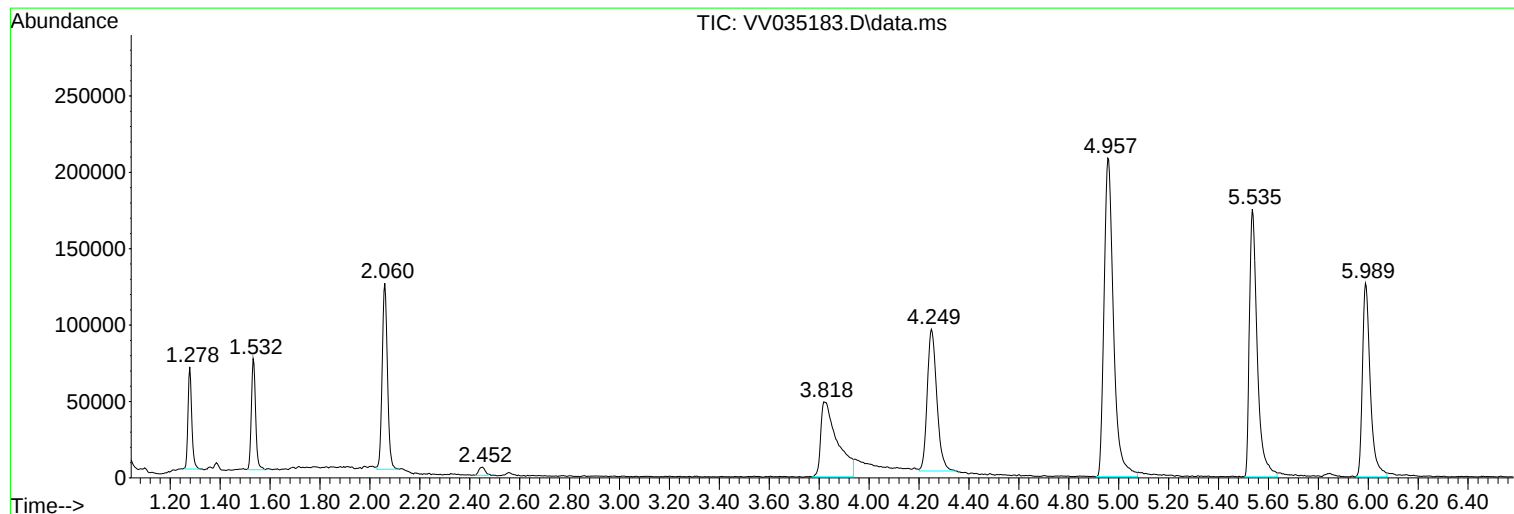

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035183.D
Acq On : 12 Apr 2024 19:03
Operator : SY/MD
Sample : P2057-10DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BM8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035183.D
Acq On : 12 Apr 2024 19:03
Operator : SY/MD
Sample : P2057-10DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BM8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc