

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
 Data File : VV035186.D
 Acq On : 12 Apr 2024 20:15
 Operator : SY/MD
 Sample : P2057-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BN4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV035186.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	91	rVB	70823	76976	12.65%	1.552%
2	1.385	101	107	117	rVB	17856	20701	3.40%	0.417%
3	1.536	146	154	166	rBV	74742	89756	14.75%	1.809%
4	1.970	282	289	297	rBV2	11512	15856	2.61%	0.320%
5	2.060	307	317	335	rVB	126972	186446	30.63%	3.759%
6	3.822	848	865	905	rBV3	71729	335208	55.07%	6.757%
7	4.249	979	998	1024	rBV2	94947	253597	41.67%	5.112%
8	4.957	1204	1218	1255	rBV2	216555	568541	93.41%	11.461%
9	5.535	1386	1398	1429	rBV	181198	396096	65.08%	7.985%
10	5.989	1527	1539	1571	rBV	130583	286302	47.04%	5.772%
11	6.918	1819	1828	1853	rBV2	40873	89358	14.68%	1.801%
12	7.246	1918	1930	1951	rBV	212347	395878	65.04%	7.981%
13	7.564	2018	2029	2046	rBV2	23455	49292	8.10%	0.994%
14	7.873	2116	2125	2127	rBV	6779	8112	1.33%	0.164%
15	7.908	2128	2136	2153	rVB3	24905	46805	7.69%	0.944%
16	8.027	2162	2173	2221	rBV	275194	608642	100.00%	12.270%
17	8.786	2397	2409	2429	rBV	302525	517951	85.10%	10.441%
18	10.153	2823	2834	2851	rBV2	106854	171850	28.23%	3.464%
19	10.326	2877	2888	2899	rBV	15226	24021	3.95%	0.484%
20	11.185	3144	3155	3178	rBV	275858	447207	73.48%	9.015%
21	11.561	3259	3272	3295	rBV	225427	371940	61.11%	7.498%




Sum of corrected areas: 4960535

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035186.D
Acq On : 12 Apr 2024 20:15
Operator : SY/MD
Sample : P2057-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

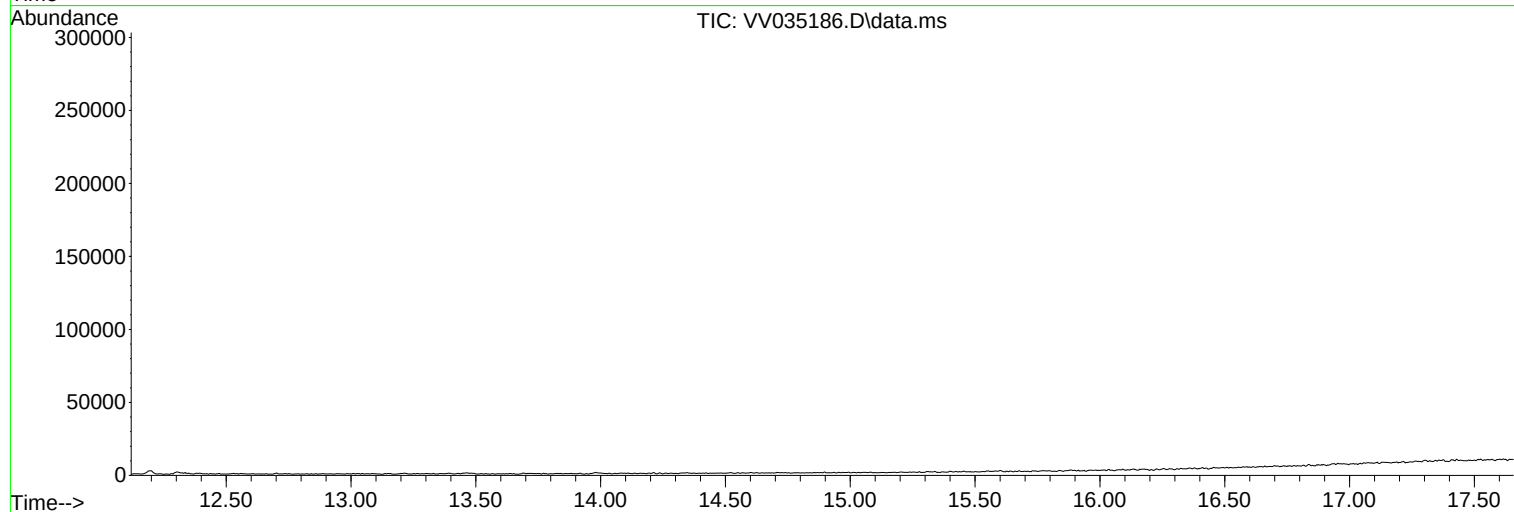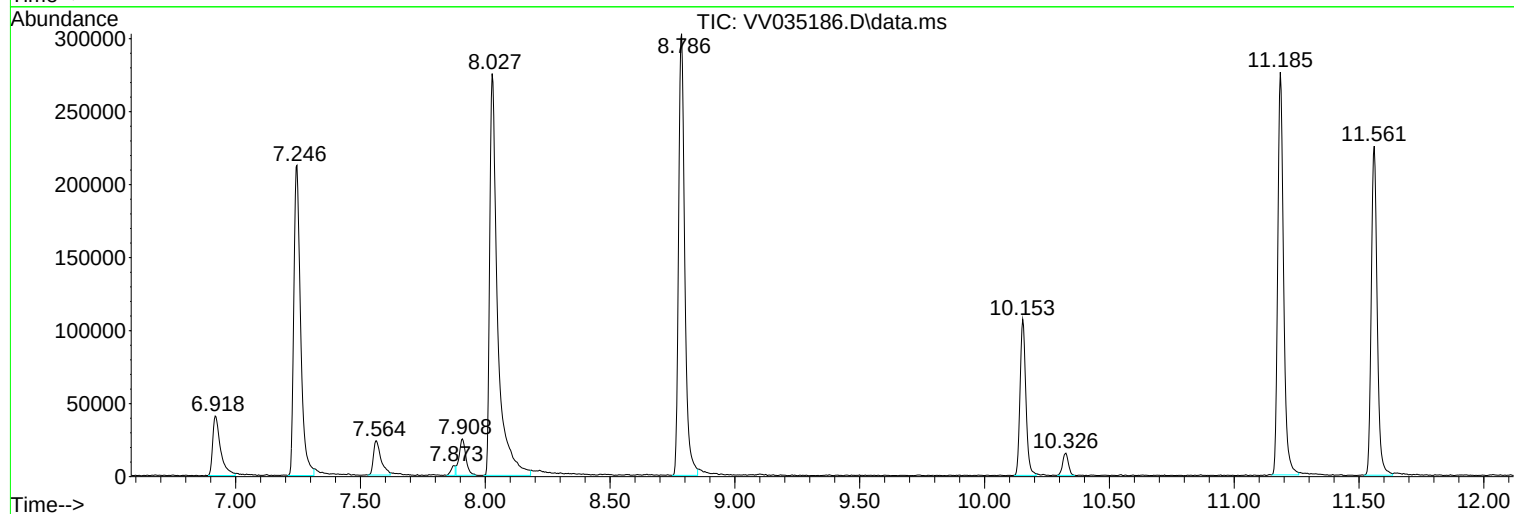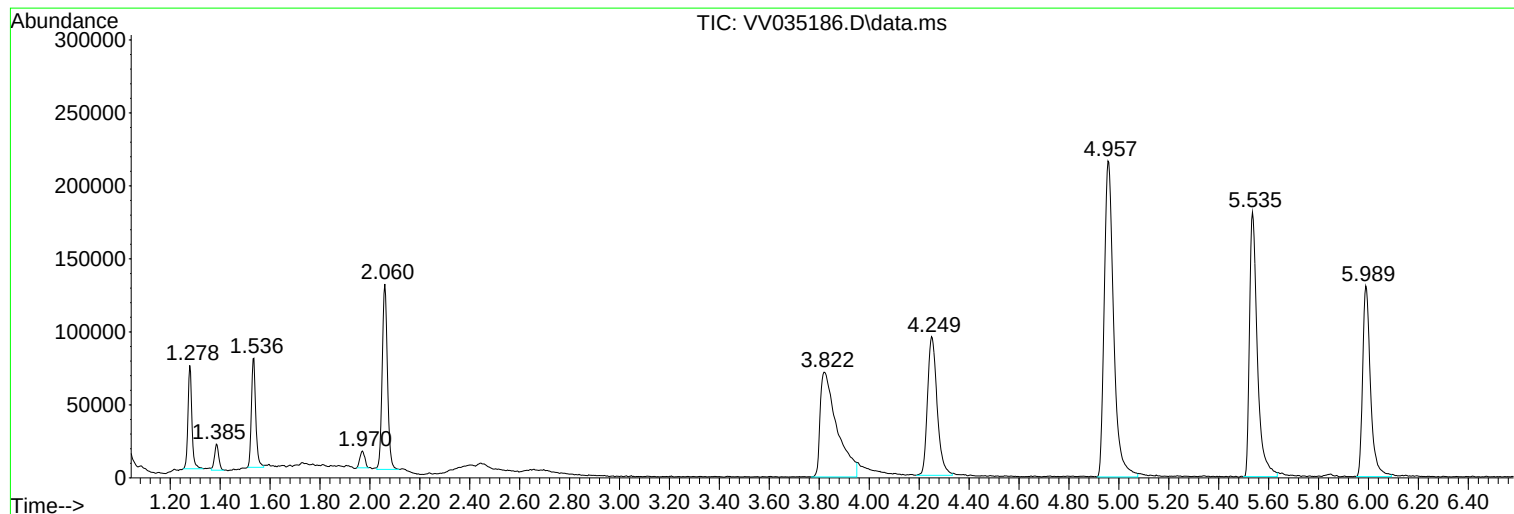

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035186.D
Acq On : 12 Apr 2024 20:15
Operator : SY/MD
Sample : P2057-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035186.D
Acq On : 12 Apr 2024 20:15
Operator : SY/MD
Sample : P2057-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc