

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
 Data File : VV035187.D
 Acq On : 12 Apr 2024 20:39
 Operator : SY/MD
 Sample : P2057-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV035187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	85	rVB	68216	71529	12.17%	1.462%
2	1.384	102	107	115	rVB	9149	10097	1.72%	0.206%
3	1.532	145	153	167	rBV	76084	92243	15.69%	1.885%
4	1.966	282	288	297	rVB2	5926	8259	1.40%	0.169%
5	2.060	307	317	331	rVB	125097	183240	31.16%	3.745%
6	3.818	848	864	913	rBV3	94133	408747	69.52%	8.354%
7	4.249	982	998	1020	rBV	95601	249312	42.40%	5.095%
8	4.957	1204	1218	1254	rBV3	217074	564836	96.06%	11.544%
9	5.535	1383	1398	1427	rBV	179147	387944	65.98%	7.929%
10	5.989	1525	1539	1570	rBV	132511	286777	48.77%	5.861%
11	6.918	1816	1828	1857	rBV2	40067	90129	15.33%	1.842%
12	7.246	1916	1930	1955	rBV	211128	397724	67.64%	8.129%
13	7.564	2019	2029	2048	rBV2	23477	48744	8.29%	0.996%
14	7.876	2115	2126	2130	rBV2	6457	10715	1.82%	0.219%
15	7.911	2133	2137	2148	rVB4	7087	10939	1.86%	0.224%
16	8.027	2164	2173	2210	rBV	270007	587986	100.00%	12.017%
17	8.786	2398	2409	2431	rBV	288051	493748	83.97%	10.091%
18	10.153	2823	2834	2853	rBV	104044	168749	28.70%	3.449%
19	10.326	2877	2888	2900	rVB2	13899	21865	3.72%	0.447%
20	11.185	3141	3155	3178	rBV	269166	432973	73.64%	8.849%
21	11.561	3259	3272	3295	rBV	222497	366262	62.29%	7.486%




Sum of corrected areas: 4892818

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035187.D
Acq On : 12 Apr 2024 20:39
Operator : SY/MD
Sample : P2057-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

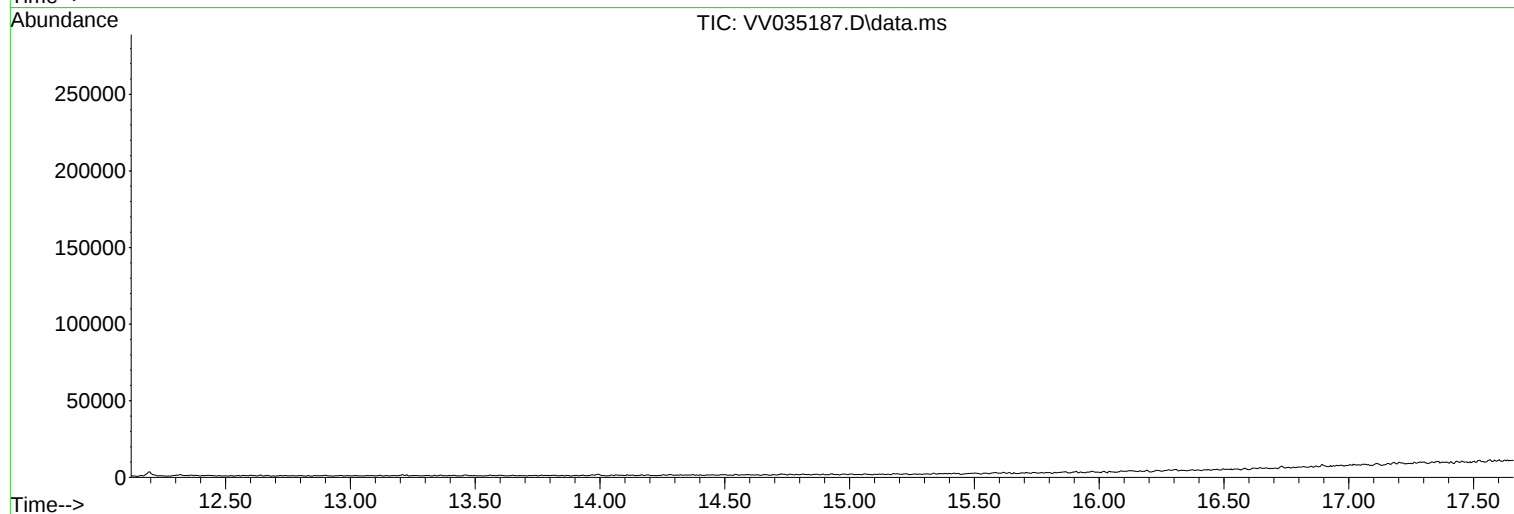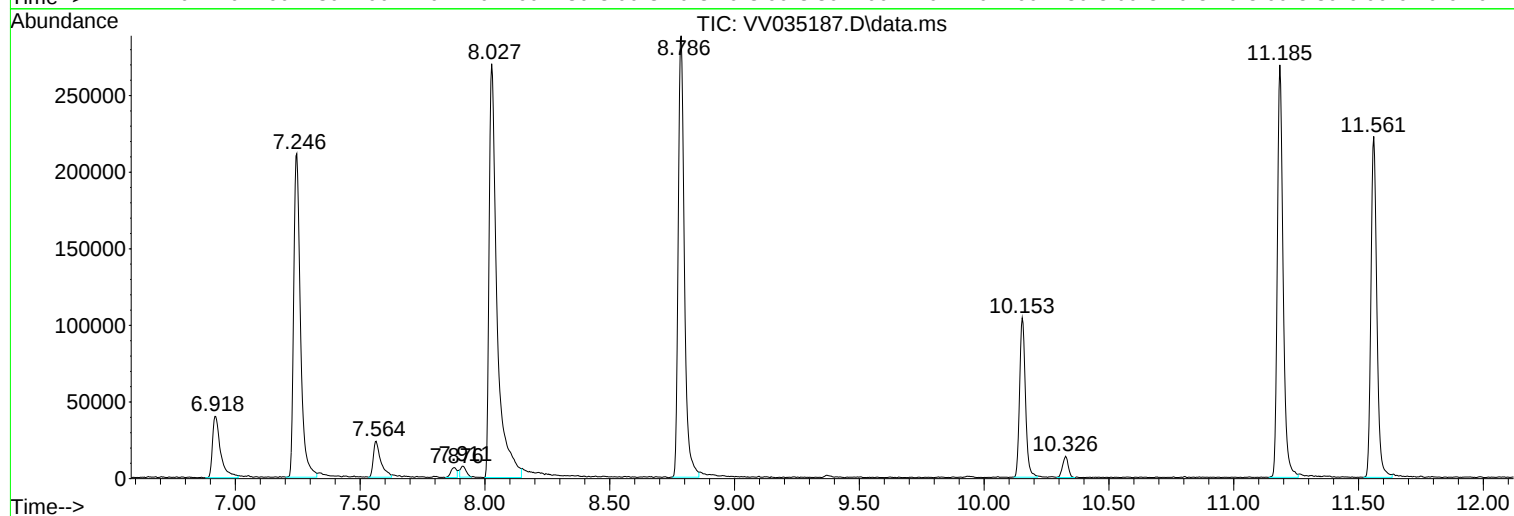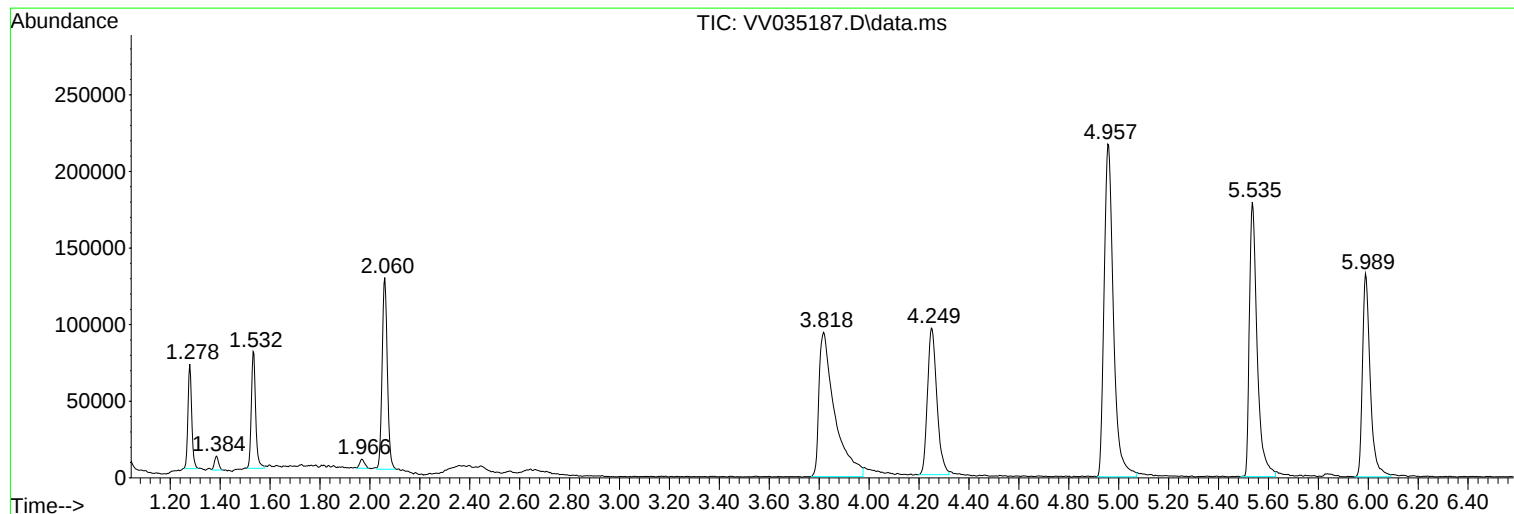

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035187.D
Acq On : 12 Apr 2024 20:39
Operator : SY/MD
Sample : P2057-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041224\
Data File : VV035187.D
Acq On : 12 Apr 2024 20:39
Operator : SY/MD
Sample : P2057-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040224WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
