


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV041319\
Data File : VV010317.D
Acq On : 13 Apr 2019 11:11
Operator : SY/MD
Sample : BFB35
Misc : 25mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB35

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR041319WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Apr 13 14:26:57 2019

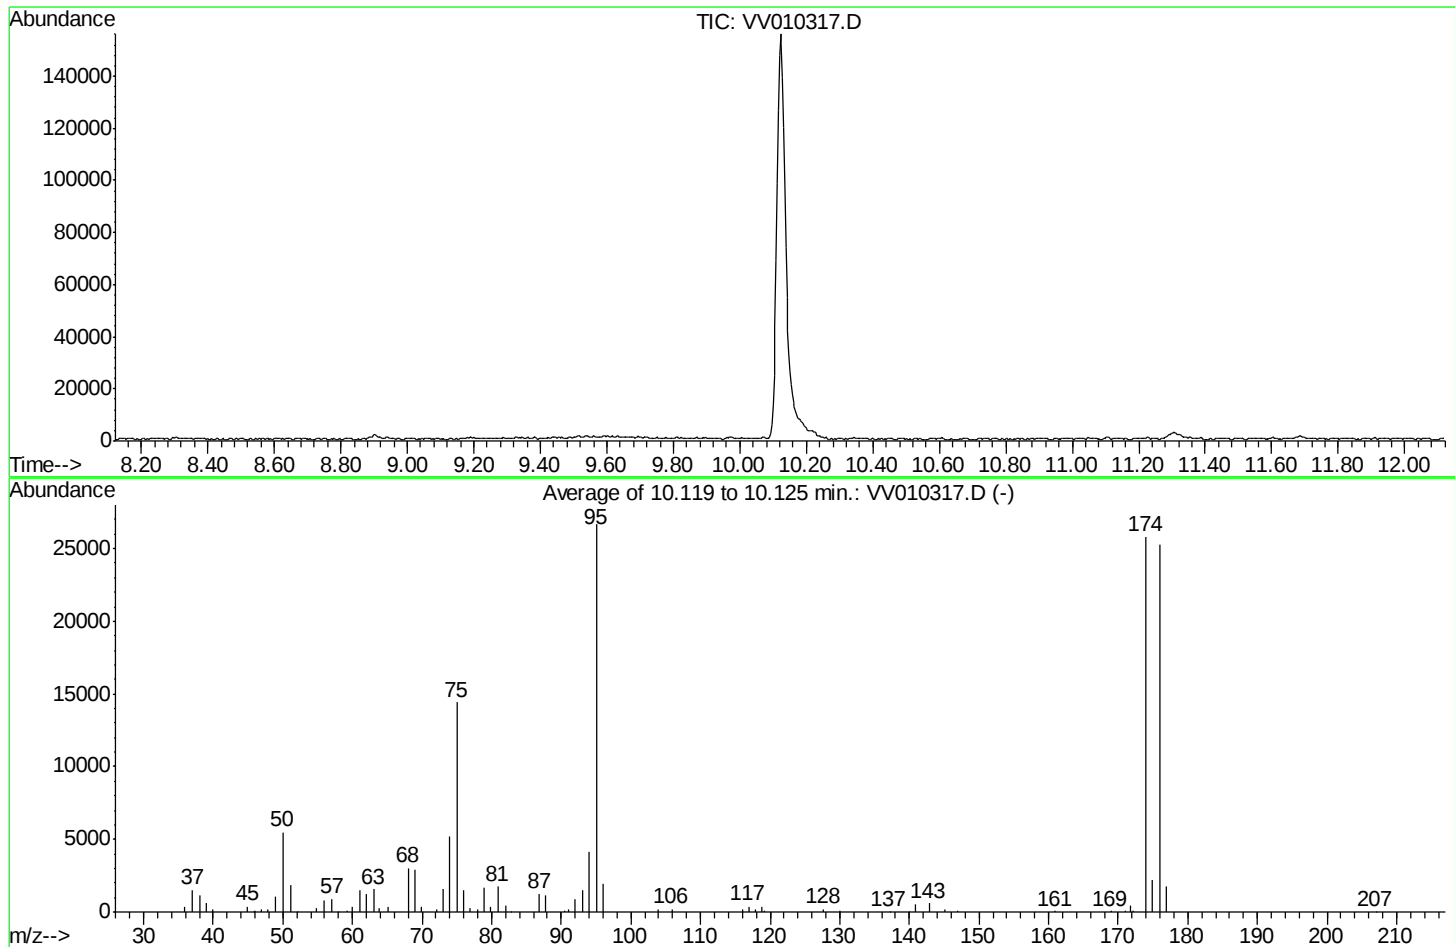

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	5493	PASS
75	95	30	80	54.0	14410	PASS
95	95	100	100	100.0	26666	PASS
96	95	5	9	7.3	1944	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	96.9	25840	PASS
175	174	5	9	8.4	2166	PASS
176	174	95	101	97.8	25274	PASS
177	176	5	9	6.9	1740	PASS

Scan 2796 (10.080 min): VV010317.D
BFB35

m/z	Abundance
35.60	110.0
40.00	270.0
40.80	108.0
44.00	467.0
169.10	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
35.90	405.0
37.00	1525.0
38.00	1212.0
39.00	480.0
40.10	501.0
44.10	471.0
44.90	358.0
45.80	108.0
46.90	174.0
48.00	205.0
48.90	1025.0
50.00	5802.0
51.10	1832.0
54.80	197.0
56.00	784.0
57.00	797.0
57.90	124.0
59.30	114.0
59.90	374.0
61.00	1489.0
62.00	1223.0
63.00	1539.0
63.90	211.0
65.20	275.0
68.00	2878.0
69.00	3073.0
69.90	308.0
72.00	221.0
73.00	1551.0
74.00	5196.0
75.00	14121.0
76.10	1537.0
76.80	264.0
77.90	131.0
78.90	1637.0
79.90	404.0
80.80	1576.0
82.00	427.0
86.90	1292.0
87.80	1053.0
90.60	103.0
90.90	134.0
91.90	882.0
93.00	1535.0
94.00	3854.0
95.00	25712.0
96.00	1870.0
103.90	147.0
105.90	236.0
116.00	165.0
116.90	347.0
117.90	132.0
118.80	259.0
127.70	166.0
130.10	108.0
137.10	134.0
139.90	109.0
141.00	514.0
142.90	571.0
145.10	200.0
146.90	159.0
169.00	194.0
171.80	429.0
172.20	338.0
174.00	24392.0
175.00	2091.0
176.00	24160.0
176.90	1683.0
207.00	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
36.00	348.0
37.00	1528.0
38.00	1183.0
39.00	657.0
40.10	469.0
44.10	436.0
44.90	405.0
46.00	115.0
46.90	151.0
47.90	183.0
48.90	1137.0
50.00	5636.0
51.10	1926.0
54.90	240.0
56.00	818.0
57.10	930.0
59.20	114.0
59.90	356.0
61.10	1563.0
62.10	1262.0
63.10	1666.0
63.90	273.0
65.20	348.0
68.00	3099.0
69.00	2933.0
69.90	363.0
72.00	223.0
73.00	1637.0
74.00	5279.0
75.00	14862.0
76.00	1536.0
76.80	292.0
77.90	155.0
78.90	1757.0
79.90	414.0
80.90	1848.0
82.00	478.0
86.90	1302.0
87.80	1166.0
90.50	125.0
90.90	134.0
92.00	918.0
93.00	1591.0
94.00	4406.0
95.00	27344.0
96.00	2001.0
103.80	172.0
105.90	230.0
116.00	154.0
116.90	419.0
117.90	129.0
118.70	353.0
127.70	200.0
130.10	107.0
141.00	524.0
142.80	624.0
145.10	208.0
161.00	108.0
169.00	237.0
171.00	167.0
171.80	490.0
174.00	26616.0
174.90	2242.0
176.00	25864.0
176.90	1707.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
36.00	231.0
37.00	1501.0
38.00	1128.0
39.00	835.0
40.00	340.0
44.00	393.0
44.90	362.0
46.00	127.0
46.90	168.0
47.80	182.0
49.00	1142.0
50.00	5042.0
51.00	1818.0
52.00	102.0
54.90	238.0
56.00	738.0
57.10	922.0
59.90	299.0
61.10	1515.0
62.00	1273.0
63.10	1503.0
63.90	269.0
65.10	375.0
68.00	3067.0
69.00	2751.0
69.90	387.0
72.10	163.0
73.00	1475.0
74.00	5012.0
75.00	14247.0
76.00	1357.0
76.90	264.0
78.00	142.0
79.00	1727.0
79.90	373.0
80.90	1850.0
81.90	489.0
82.80	130.0
86.90	1152.0
87.80	1242.0
90.50	107.0
91.00	169.0
92.00	864.0
93.00	1484.0
94.00	4221.0
95.00	26944.0
96.00	1963.0
103.80	210.0
105.90	195.0
116.00	122.0
116.90	336.0
118.00	172.0
118.70	374.0
119.20	235.0
127.70	182.0
140.90	540.0
142.80	648.0
145.10	148.0
161.00	111.0
169.00	267.0
171.00	182.0
171.80	498.0
174.00	26512.0
174.90	2166.0
176.00	25800.0
177.00	1832.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35