
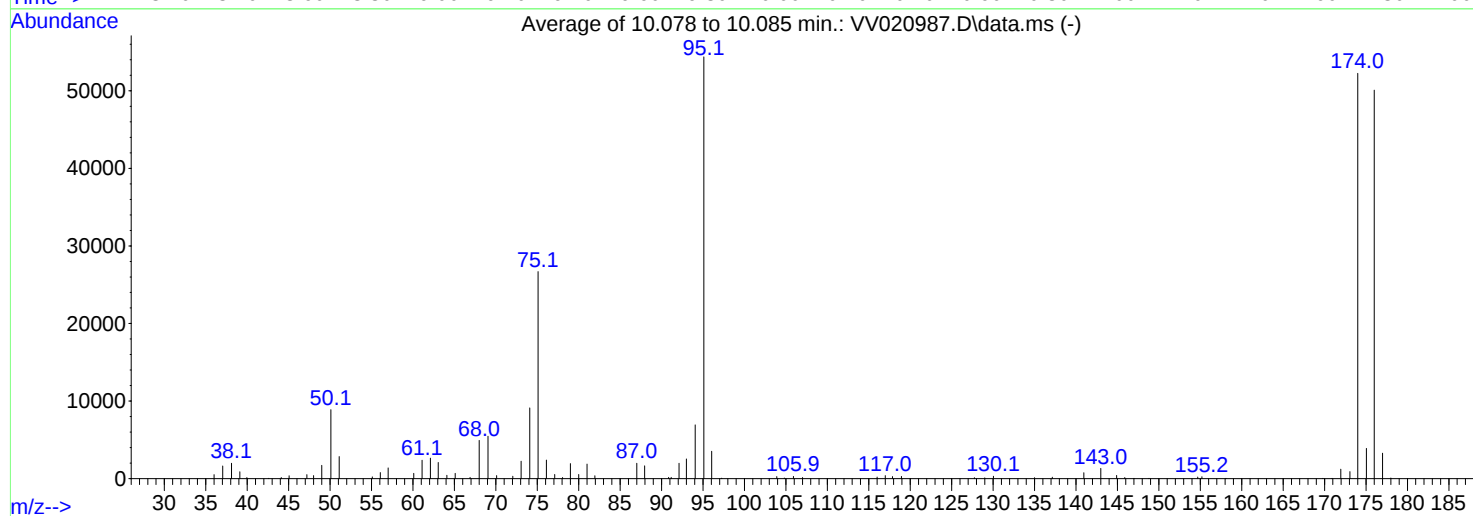


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041321\
Data File : VV020987.D
Acq On : 13 Apr 2021 09:00
Operator : SY/MD
Sample : BFB75
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB75

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM041321WMA.M
Title : VOC Analysis
Last Update : Wed Apr 14 03:24:48 2021

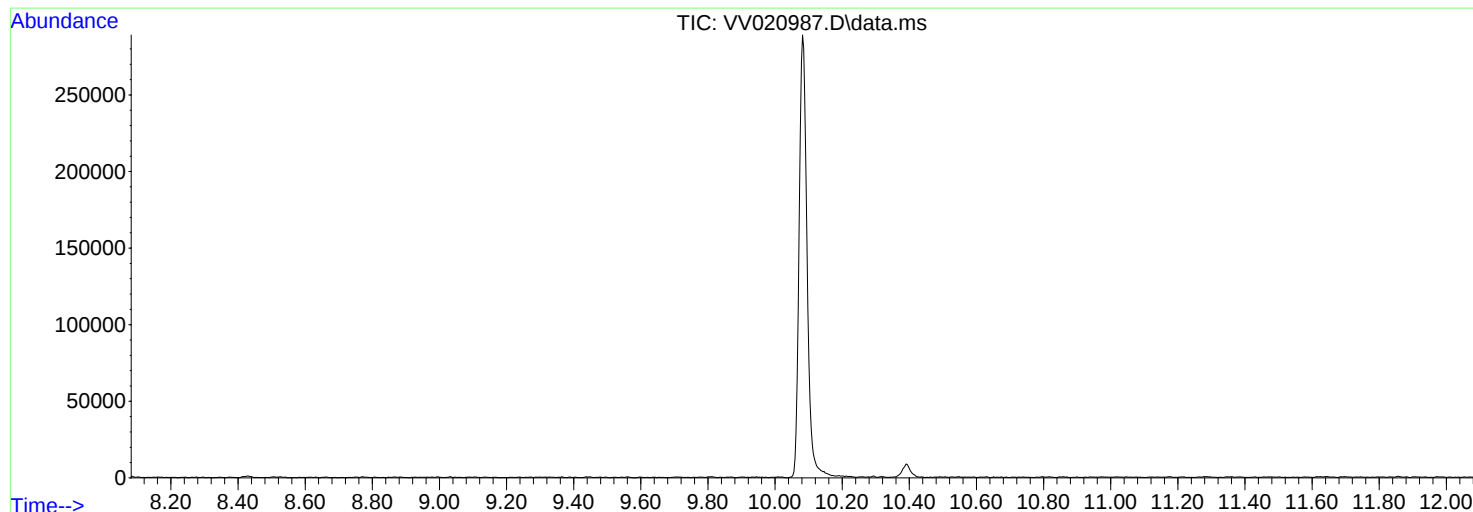

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	8883	PASS
75	95	30	80	49.1	26685	PASS
95	95	100	100	100.0	54376	PASS
96	95	5	9	6.5	3527	PASS
173	174	0.00	2	1.7	902	PASS
174	95	50	120	96.1	52253	PASS
175	174	5	9	7.5	3908	PASS
176	174	95	101	95.8	50080	PASS
177	176	5	9	6.6	3282	PASS

Scan 2801 (10.046 min): VV020987.D\data.ms
BFB75

m/z	Abundance
39.90	178.0
44.10	313.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.00	445.0
37.00	1707.0
38.10	1739.0
39.10	963.0
40.00	276.0
44.10	407.0
45.00	244.0
47.20	465.0
48.00	354.0
49.00	1680.0
50.10	8804.0
51.10	2826.0
55.10	188.0
56.00	802.0
57.00	1369.0
60.10	685.0
61.10	2155.0
62.10	2438.0
63.00	2036.0
64.10	431.0
65.10	592.0
66.90	177.0
68.00	4749.0
69.00	5135.0
70.10	310.0
72.10	293.0
73.10	2128.0
74.10	8669.0
75.10	25240.0
76.10	2568.0
77.10	593.0
78.10	128.0
79.00	1809.0
80.00	467.0
81.00	1882.0
81.90	320.0
87.00	1890.0
87.90	1714.0
90.80	133.0
91.20	143.0
92.10	2036.0
93.00	2526.0
94.00	6740.0
95.10	53368.0
96.00	3716.0
103.90	239.0
104.80	171.0
105.90	356.0
107.00	139.0
116.10	317.0
116.90	393.0
117.80	233.0
118.90	309.0
129.00	154.0
130.10	355.0
135.00	116.0
137.20	106.0
140.90	769.0
143.00	1317.0
144.90	379.0
145.90	183.0
154.70	222.0
155.20	295.0
169.80	106.0
170.90	139.0
172.00	1211.0
173.00	688.0
174.00	49568.0
175.10	4023.0
176.00	48344.0
177.00	3262.0
178.00	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.00	551.0
37.00	1639.0
38.10	2075.0
39.10	928.0
40.00	356.0
44.20	466.0
45.10	366.0
47.20	567.0
48.00	438.0
49.00	1784.0
50.10	9346.0
51.10	2975.0
55.10	234.0
56.10	782.0
57.00	1450.0
60.10	697.0
61.10	2447.0
62.10	2752.0
63.00	2146.0
64.10	497.0
65.10	669.0
66.90	138.0
68.00	5104.0
69.10	5692.0
70.10	387.0
72.10	337.0
73.00	2317.0
74.10	9480.0
75.10	27568.0
76.10	2465.0
77.10	585.0
78.00	105.0
79.00	2000.0
80.00	523.0
81.00	1884.0
81.90	375.0
87.00	2008.0
88.00	1768.0
90.80	164.0
91.20	175.0
92.10	2065.0
93.00	2571.0
94.00	7183.0
95.10	55896.0
96.10	3611.0
97.30	109.0
103.90	290.0
104.80	106.0
105.90	294.0
107.00	167.0
116.00	158.0
117.00	390.0
117.90	281.0
118.90	270.0
127.70	144.0
129.00	134.0
130.10	349.0
135.00	131.0
137.10	208.0
141.00	754.0
143.00	1439.0
144.90	434.0
145.90	139.0
154.70	242.0
155.20	260.0
172.00	1257.0
173.10	909.0
174.00	53864.0
175.00	4060.0
176.00	51680.0
177.00	3366.0
178.00	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.00	535.0
37.10	1547.0
38.10	2112.0
39.10	746.0
40.00	318.0
42.60	104.0
44.20	500.0
45.10	504.0
47.20	531.0
48.00	381.0
49.00	1663.0
50.10	8498.0
51.10	2750.0
55.10	263.0
56.10	786.0
57.00	1359.0
60.10	686.0
61.10	2509.0
62.10	2747.0
63.10	2089.0
64.10	401.0
65.10	791.0
66.90	156.0
68.00	4932.0
69.10	5558.0
70.10	500.0
72.00	329.0
73.00	2317.0
74.10	9223.0
75.10	27248.0
76.10	2149.0
77.10	453.0
78.00	208.0
79.00	2019.0
80.00	638.0
81.00	1842.0
82.00	447.0
87.00	2048.0
88.00	1493.0
90.90	187.0
91.00	187.0
92.10	1820.0
93.00	2542.0
94.10	6882.0
95.10	53864.0
96.10	3253.0
97.20	110.0
103.90	285.0
105.90	226.0
107.00	130.0
115.90	121.0
117.10	372.0
117.90	277.0
119.00	285.0
127.80	250.0
130.00	259.0
135.00	152.0
137.10	234.0
140.90	759.0
143.00	1203.0
144.90	417.0
145.90	112.0
147.00	105.0
148.80	125.0
154.70	147.0
155.20	202.0
158.10	109.0
171.90	1166.0
173.10	1110.0
174.00	53328.0
175.00	3641.0
176.00	50216.0
177.00	3219.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75