

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041323\
 Data File : VW030544.D
 Acq On : 13 Apr 2023 14:43
 Operator : SY/MD
 Sample : 02275-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDY7

Quant Time: Apr 14 05:20:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 14 05:16:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	84585	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.796	117	86102	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	39487	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	36007	6.427	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	128.600%	
7) Chloroethane-d5	1.536	69	29764	5.475	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	109.400%	
11) 1,1-Dichloroethene-d2	2.066	63	51923	3.906	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	78.200%	
20) 2-Butanone-d5	3.809	46	94463	65.238	ug/L	-0.03
Spiked Amount	50.000	Range 40 - 130	Recovery	=	130.480%#	
24) Chloroform-d	4.265	84	62763	4.629	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.600%	
26) 1,2-Dichloroethane-d4	4.957	65	37753	5.902	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	118.000%	
32) Benzene-d6	4.973	84	109228	4.502	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.000%	
36) 1,2-Dichloropropane-d6	5.998	67	35781	4.710	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	94.200%	
41) Toluene-d8	7.252	98	89655	4.024	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	80.400%	
43) trans-1,3-Dichloroprop...	7.564	79	12365	4.323	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	86.400%	
46) 2-Hexanone-d5	8.034	63	67416	58.662	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	117.320%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	32766	5.473	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	109.400%	
66) 1,2-Dichlorobenzene-d4	11.571	152	35334	5.007	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	100.200%	
Target Compounds						Qvalue
13) Acetone	2.137	43	2657	1.919	ug/L	64
42) Toluene	7.330	91	16417	0.504	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030544.D
Acq On : 13 Apr 2023 14:43
Operator : SY/MD
Sample : 02275-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY7

Quant Time: Apr 14 05:20:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 14 05:16:37 2023
Response via : Initial Calibration

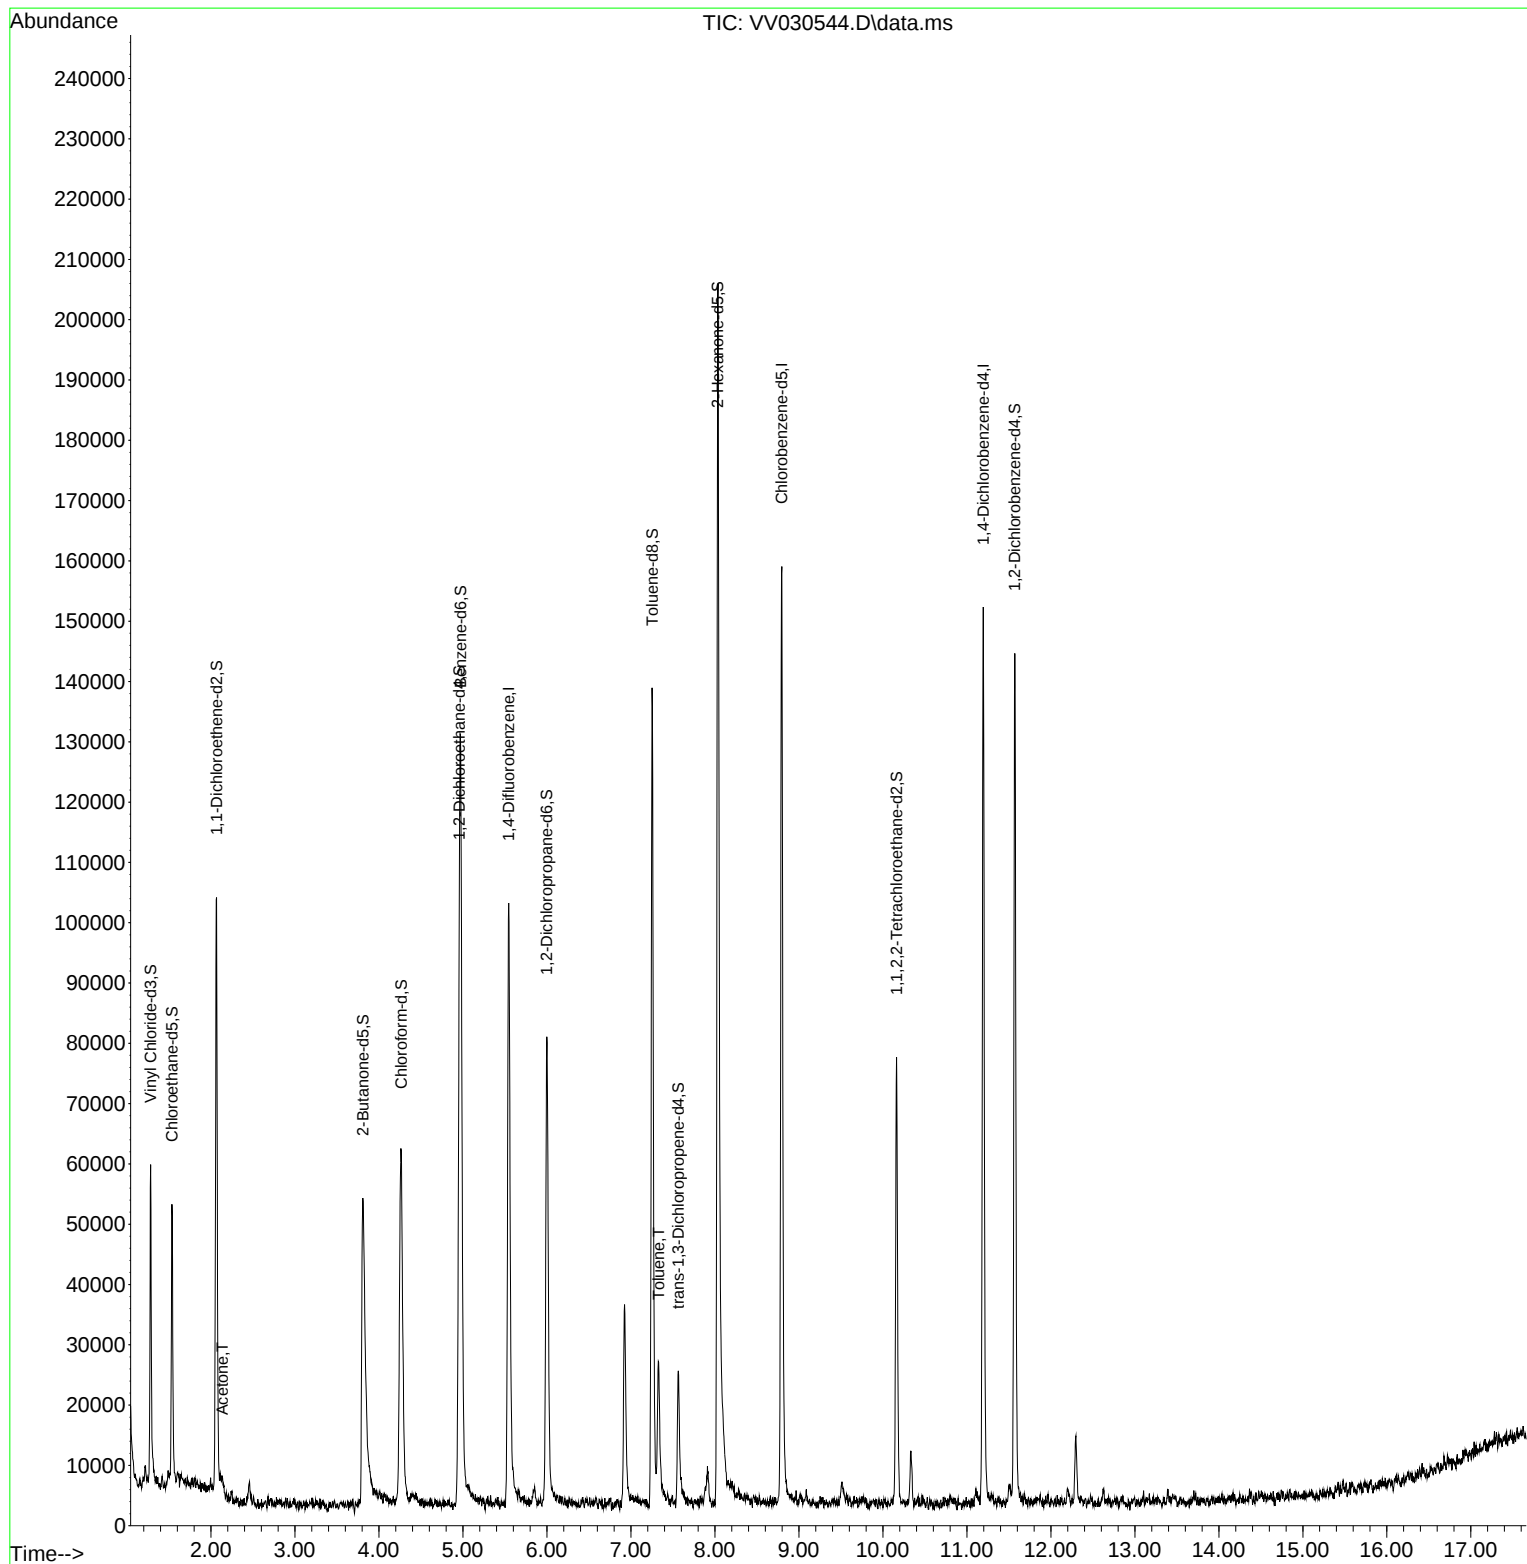

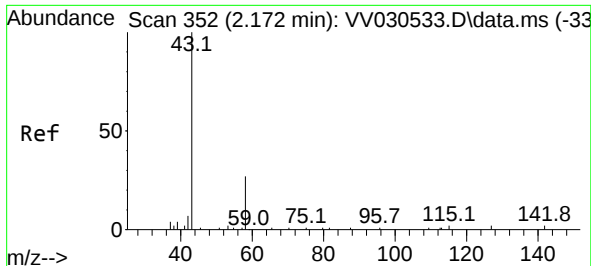

#13

Acetone

Concen: 1.919 ug/L

RT: 2.137 min Scan# 341

Delta R.T. -0.035 min

Lab File: VV030544.D

Acq: 13 Apr 2023 14:43

Instrument :

MSVOA_V

ClientSampleId :





BHDY7

Tgt Ion: 43 Resp: 2657

Ion Ratio Lower Upper

43 100

58 37.3 0.0 40.8

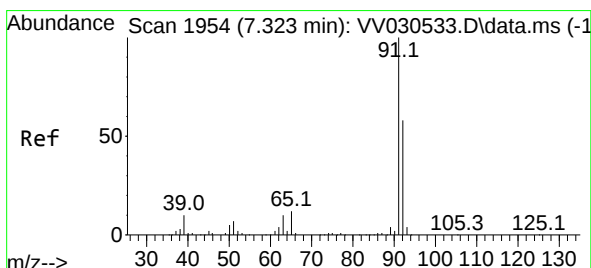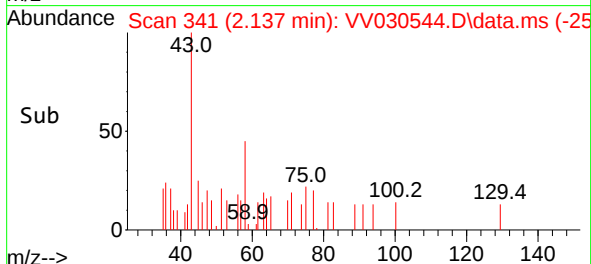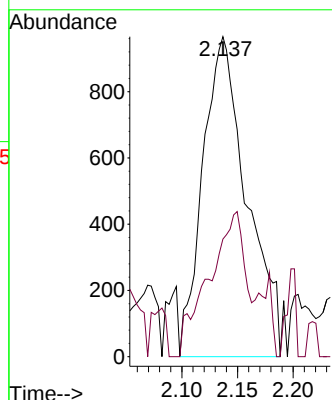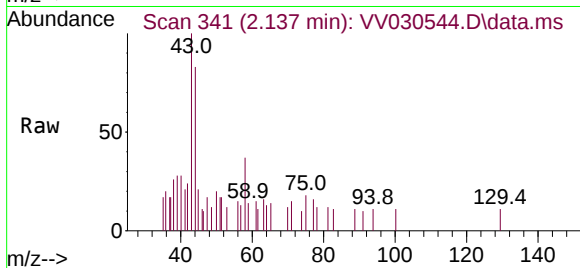

#42

Toluene

Concen: 0.504 ug/L

RT: 7.330 min Scan# 1956

Delta R.T. 0.006 min

Lab File: VV030544.D

Acq: 13 Apr 2023 14:43

Tgt Ion: 91 Resp: 16417

Ion Ratio Lower Upper

91 100

92 54.7 40.4 75.0

