

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
 Data File : VV030535.D
 Acq On : 13 Apr 2023 11:10
 Operator : SY/MD
 Sample : 02250-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDx7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030535.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	91	rBV	77458	86274	19.17%	2.282%
2	1.535	146	154	166	rBV	61169	73663	16.37%	1.949%
3	2.059	307	317	328	rBV	139615	203600	45.24%	5.386%
4	2.455	425	440	449	rBV2	13804	26085	5.80%	0.690%
5	3.844	858	872	873	rBV	21460	37294	8.29%	0.987%
6	4.259	986	1001	1020	rBV2	83277	209124	46.46%	5.533%
7	4.966	1203	1221	1245	rBV3	175701	450072	100.00%	11.907%
8	5.542	1386	1400	1420	rBV	147319	317393	70.52%	8.397%
9	5.998	1530	1542	1564	rBV2	102599	217836	48.40%	5.763%
10	6.921	1819	1829	1845	rBV2	43763	82249	18.27%	2.176%
11	7.252	1917	1932	1945	rBV	196245	350554	77.89%	9.274%
12	7.326	1946	1955	1975	rVB	65582	125775	27.95%	3.327%
13	7.564	2019	2029	2041	rBV2	27522	50164	11.15%	1.327%
14	8.040	2165	2177	2210	rBV	150315	353926	78.64%	9.363%
15	8.792	2400	2411	2430	rBV	231762	392244	87.15%	10.377%
16	9.509	2625	2634	2639	rBV	4871	7026	1.56%	0.186%
17	10.162	2826	2837	2851	rBV	73377	118123	26.25%	3.125%
18	10.332	2884	2890	2897	rVB5	4896	6098	1.35%	0.161%
19	11.194	3146	3158	3179	rBV	223132	357014	79.32%	9.445%
20	11.570	3263	3275	3293	rVB	181764	297895	66.19%	7.881%
21	12.300	3492	3502	3511	rBV	9438	17472	3.88%	0.462%




Sum of corrected areas: 3779881

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030535.D
Acq On : 13 Apr 2023 11:10
Operator : SY/MD
Sample : 02250-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

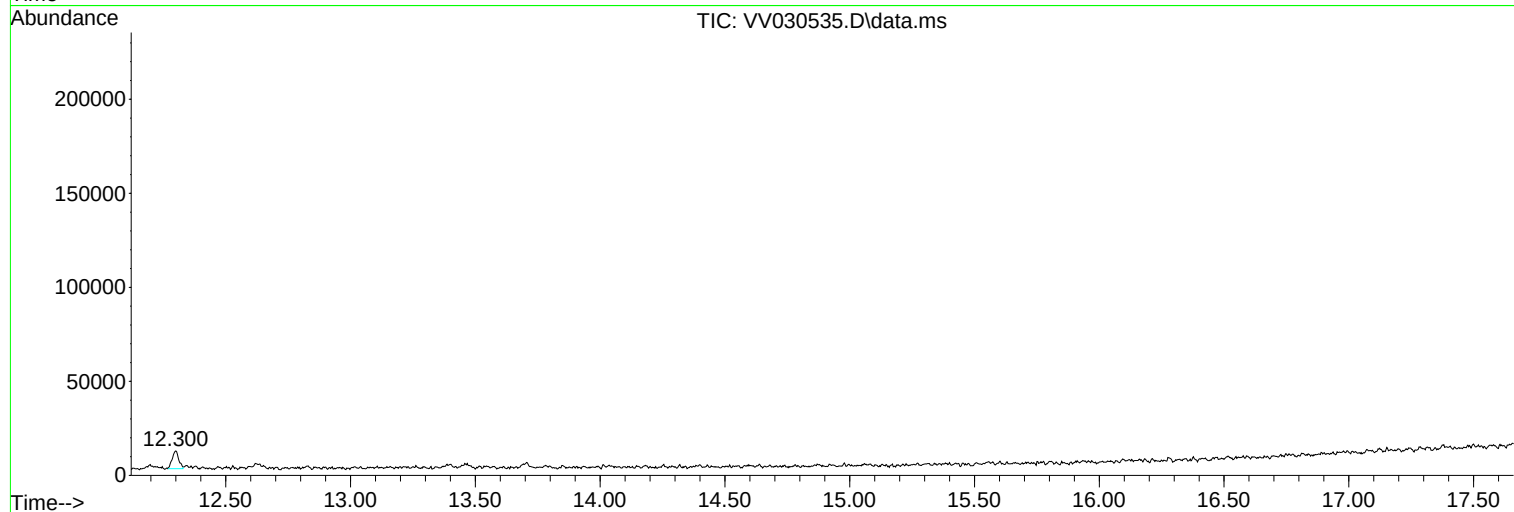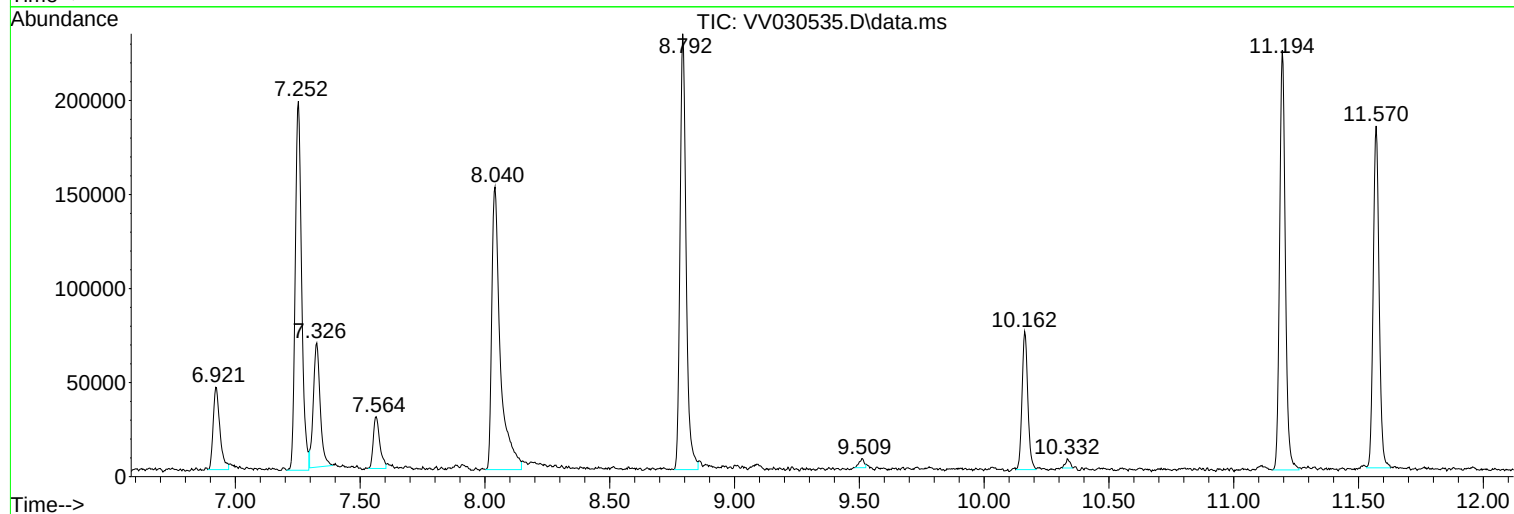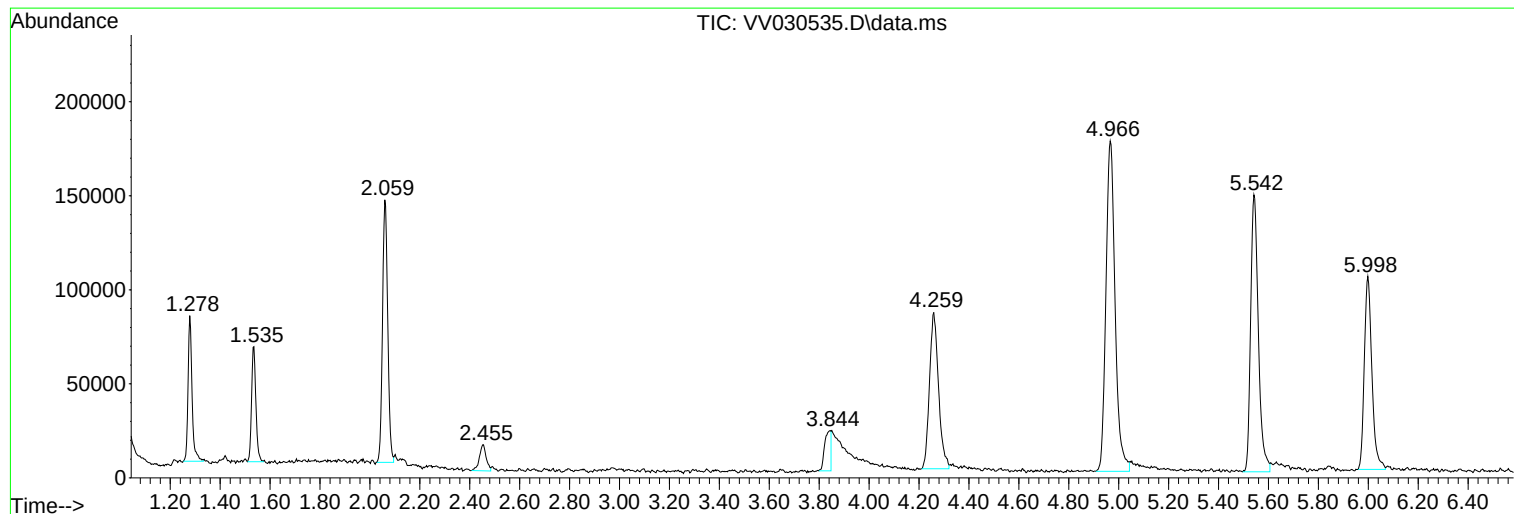

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030535.D
Acq On : 13 Apr 2023 11:10
Operator : SY/MD
Sample : 02250-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030535.D
Acq On : 13 Apr 2023 11:10
Operator : SY/MD
Sample : 02250-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------