

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
 Data File : VV030537.D
 Acq On : 13 Apr 2023 11:59
 Operator : SY/MD
 Sample : 02250-03DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDx4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030537.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rVB	47726	52411	12.52%	1.297%
2	1.539	147	155	166	rBV	47632	57706	13.79%	1.428%
3	2.066	307	319	335	rBV2	112710	182945	43.71%	4.527%
4	2.455	430	440	448	rBV5	6001	10333	2.47%	0.256%
5	3.114	637	645	647	rBV7	4647	4492	1.07%	0.111%
6	3.821	853	865	891	rBV3	42063	146760	35.06%	3.631%
7	4.262	984	1002	1023	rBV2	78305	204327	48.81%	5.056%
8	4.969	1207	1222	1243	rBV3	162091	418578	100.00%	10.357%
9	5.545	1386	1401	1421	rBV	147795	315104	75.28%	7.797%
10	5.844	1481	1494	1508	rBV	165603	333331	79.63%	8.248%
11	5.998	1529	1542	1563	rBV	99224	212560	50.78%	5.259%
12	6.924	1819	1830	1846	rBV	42401	83265	19.89%	2.060%
13	7.252	1917	1932	1954	rBV	185573	342649	81.86%	8.478%
14	7.564	2017	2029	2041	rBV	26152	49244	11.76%	1.218%
15	7.915	2120	2138	2155	rBV3	58545	114912	27.45%	2.843%
16	8.037	2163	2176	2208	rBV	161763	344847	82.39%	8.532%
17	8.792	2398	2411	2429	rBV	225233	386183	92.26%	9.555%
18	10.162	2826	2837	2851	rBV2	70804	119292	28.50%	2.952%
19	10.336	2882	2891	2902	rVB7	5477	10440	2.49%	0.258%
20	11.194	3147	3158	3172	rBV	216709	344812	82.38%	8.532%
21	11.506	3246	3255	3263	rBV	7151	15404	3.68%	0.381%
22	11.570	3263	3275	3290	rVB	179569	291980	69.76%	7.224%




Sum of corrected areas: 4041575

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030537.D
Acq On : 13 Apr 2023 11:59
Operator : SY/MD
Sample : 02250-03DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

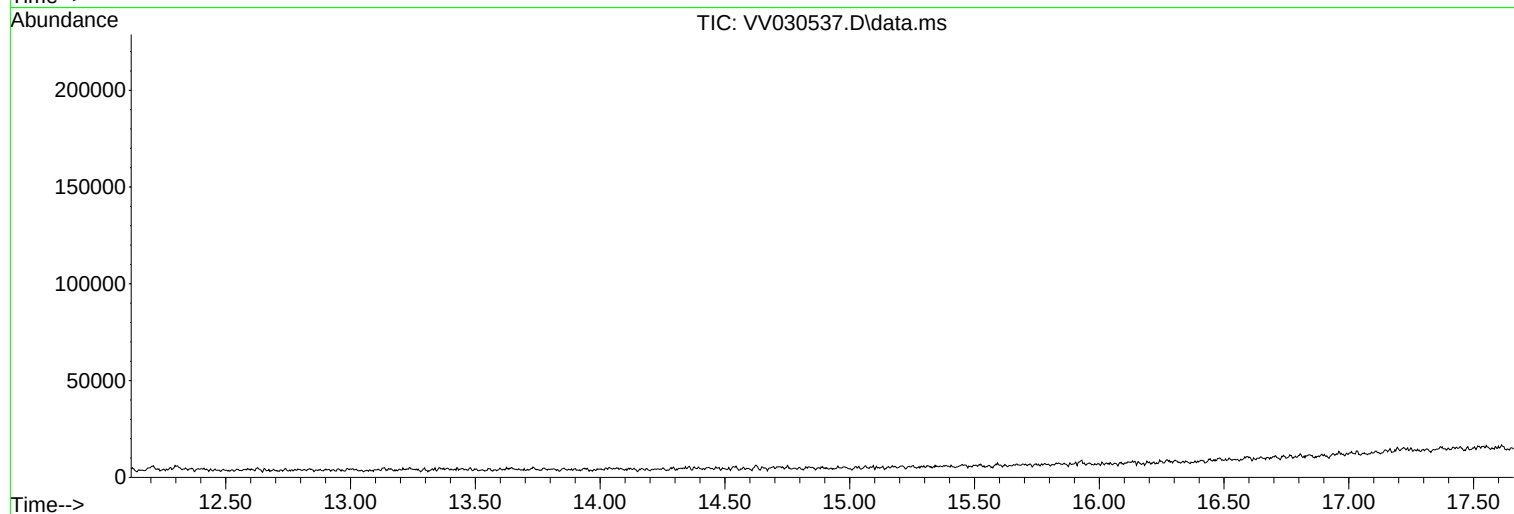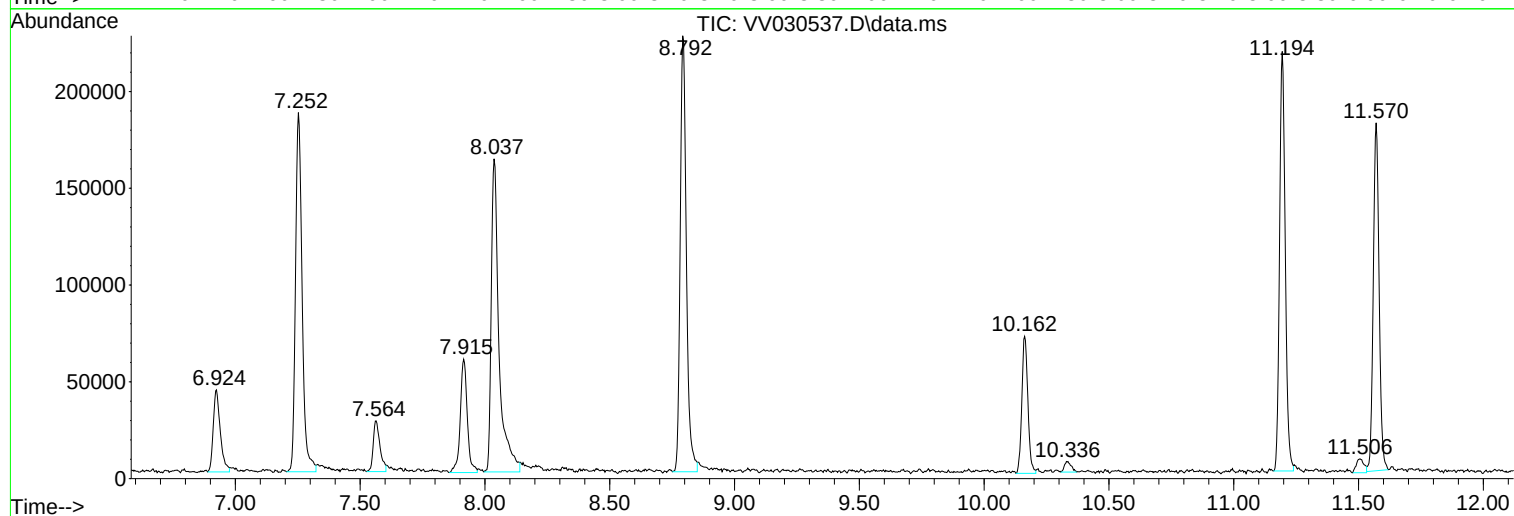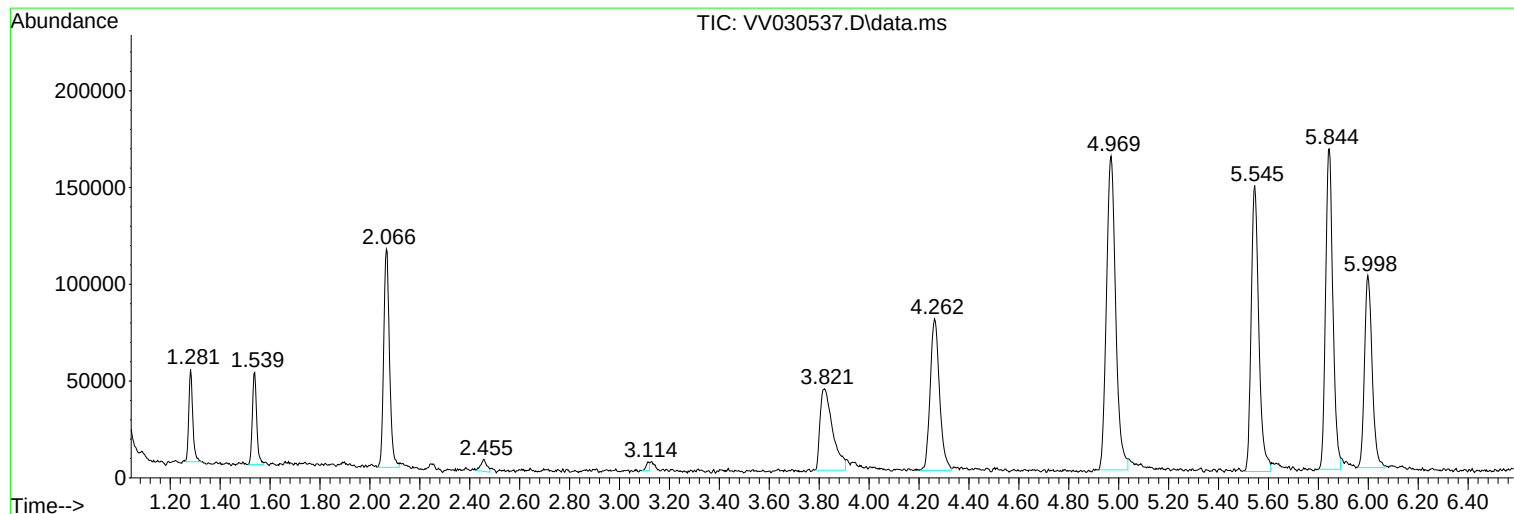

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030537.D
Acq On : 13 Apr 2023 11:59
Operator : SY/MD
Sample : 02250-03DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030537.D
Acq On : 13 Apr 2023 11:59
Operator : SY/MD
Sample : 02250-03DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHD4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------