

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
 Data File : VV030538.D
 Acq On : 13 Apr 2023 12:24
 Operator : SY/MD
 Sample : 02250-05DL 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHD6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	93	rVB	46587	55053	12.80%	1.232%
2	1.535	147	154	165	rBV	50210	58460	13.59%	1.309%
3	2.069	309	320	335	rBV3	244097	418647	97.33%	9.371%
4	2.458	429	441	452	rVB10	5740	12017	2.79%	0.269%
5	3.124	636	648	662	rBV2	30411	64084	14.90%	1.434%
6	3.831	857	868	888	rBV2	35443	131269	30.52%	2.938%
7	4.262	986	1002	1022	rBV2	76628	202245	47.02%	4.527%
8	4.526	1069	1084	1098	rVB5	9608	26156	6.08%	0.585%
9	4.969	1205	1222	1242	rBV3	163523	430149	100.00%	9.629%
10	5.545	1388	1401	1422	rBV	148196	315908	73.44%	7.071%
11	5.844	1480	1494	1511	rBV	202528	411345	95.63%	9.208%
12	5.998	1529	1542	1558	rBV	104088	216014	50.22%	4.835%
13	6.924	1821	1830	1846	rBV2	42380	81516	18.95%	1.825%
14	7.252	1920	1932	1947	rBV	186092	331767	77.13%	7.426%
15	7.564	2016	2029	2043	rBV	27594	53776	12.50%	1.204%
16	7.915	2126	2138	2149	rBV2	54840	97533	22.67%	2.183%
17	8.040	2166	2177	2206	rBV	179352	387271	90.03%	8.669%
18	8.796	2399	2412	2436	rBV	227348	393791	91.55%	8.815%
19	10.165	2825	2838	2852	rBV	78344	129831	30.18%	2.906%
20	11.194	3147	3158	3173	rBV	219098	354208	82.35%	7.929%
21	11.570	3264	3275	3291	rBV	185741	296403	68.91%	6.635%




Sum of corrected areas: 4467443

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030538.D
Acq On : 13 Apr 2023 12:24
Operator : SY/MD
Sample : 02250-05DL 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHD6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

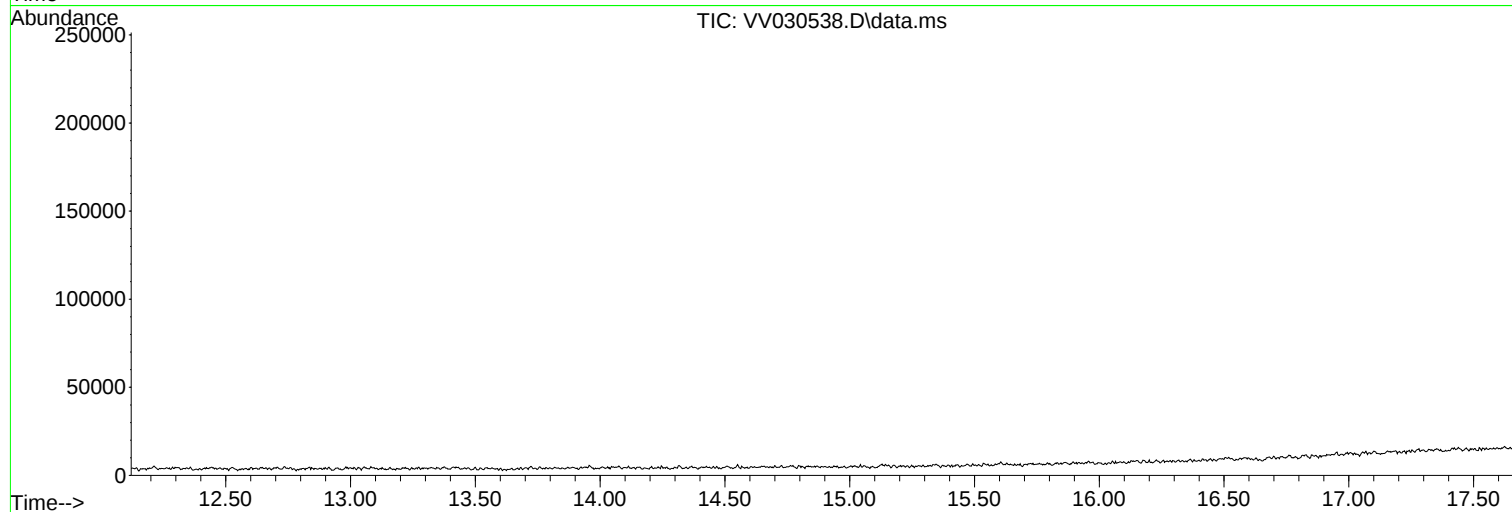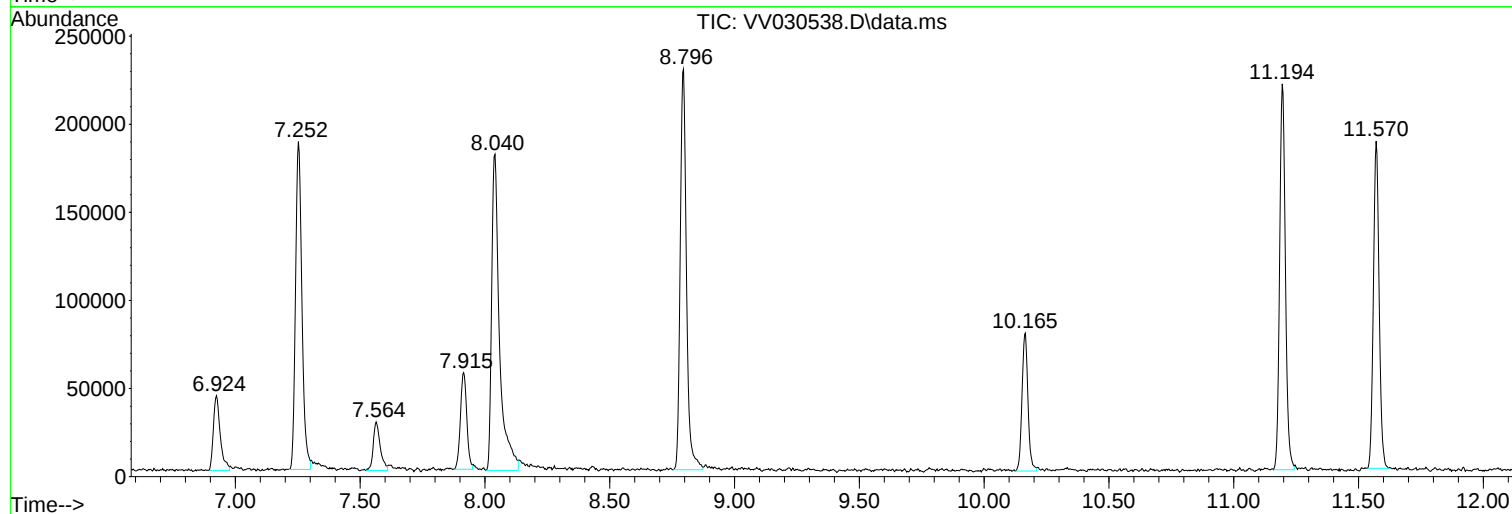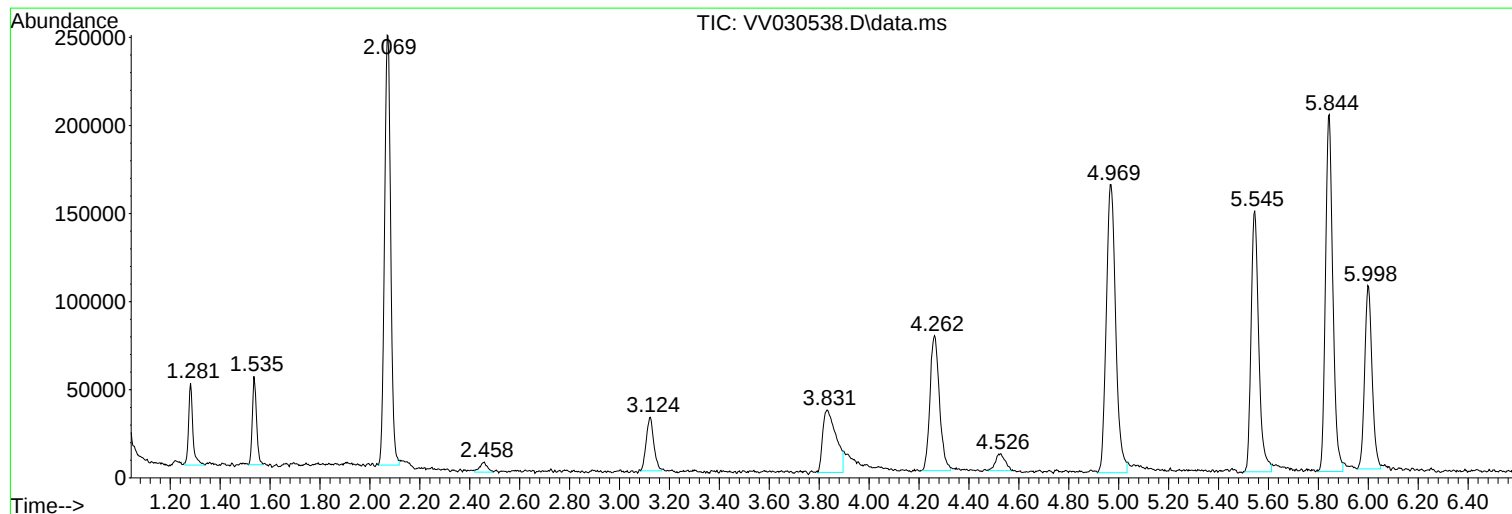

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030538.D
Acq On : 13 Apr 2023 12:24
Operator : SY/MD
Sample : 02250-05DL 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHD6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030538.D
Acq On : 13 Apr 2023 12:24
Operator : SY/MD
Sample : 02250-05DL 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHD6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------