

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
 Data File : VV030539.D
 Acq On : 13 Apr 2023 12:46
 Operator : SY/MD
 Sample : 02254-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030539.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	62	rBV6	4348	5352	1.22%	0.148%
2	1.281	69	75	86	rBV	62964	68783	15.62%	1.908%
3	1.535	148	154	166	rVB	57182	67802	15.40%	1.881%
4	2.063	308	318	336	rVV	119194	179843	40.84%	4.989%
5	3.834	858	869	898	rBV2	30244	137229	31.17%	3.807%
6	4.262	981	1002	1025	rBV2	81858	210977	47.91%	5.853%
7	4.973	1205	1223	1248	rBV2	167942	440321	100.00%	12.215%
8	5.545	1387	1401	1419	rBV	131732	279848	63.56%	7.763%
9	6.001	1528	1543	1563	rBV	99623	215394	48.92%	5.975%
10	6.924	1819	1830	1846	rBV2	42308	83392	18.94%	2.313%
11	7.252	1918	1932	1951	rBV	178645	328191	74.53%	9.104%
12	7.564	2021	2029	2046	rBV2	25790	46694	10.60%	1.295%
13	8.040	2167	2177	2208	rBV	188123	410942	93.33%	11.400%
14	8.796	2401	2412	2436	rBV	198837	346944	78.79%	9.625%
15	9.088	2495	2503	2507	rBV7	4149	6648	1.51%	0.184%
16	10.162	2826	2837	2858	rVB	78730	131888	29.95%	3.659%
17	10.339	2884	2892	2899	rBV9	3059	4567	1.04%	0.127%
18	11.107	3122	3131	3136	rBV10	3367	4875	1.11%	0.135%
19	11.194	3144	3158	3175	rBV	197823	316150	71.80%	8.770%
20	11.506	3247	3255	3260	rBV	4385	7213	1.64%	0.200%
21	11.570	3264	3275	3289	rVV	178811	285387	64.81%	7.917%
22	12.297	3491	3501	3513	rBV10	12660	21143	4.80%	0.587%
23	13.393	3832	3842	3845	rBV10	3064	5158	1.17%	0.143%




Sum of corrected areas: 3604741

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030539.D
Acq On : 13 Apr 2023 12:46
Operator : SY/MD
Sample : 02254-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

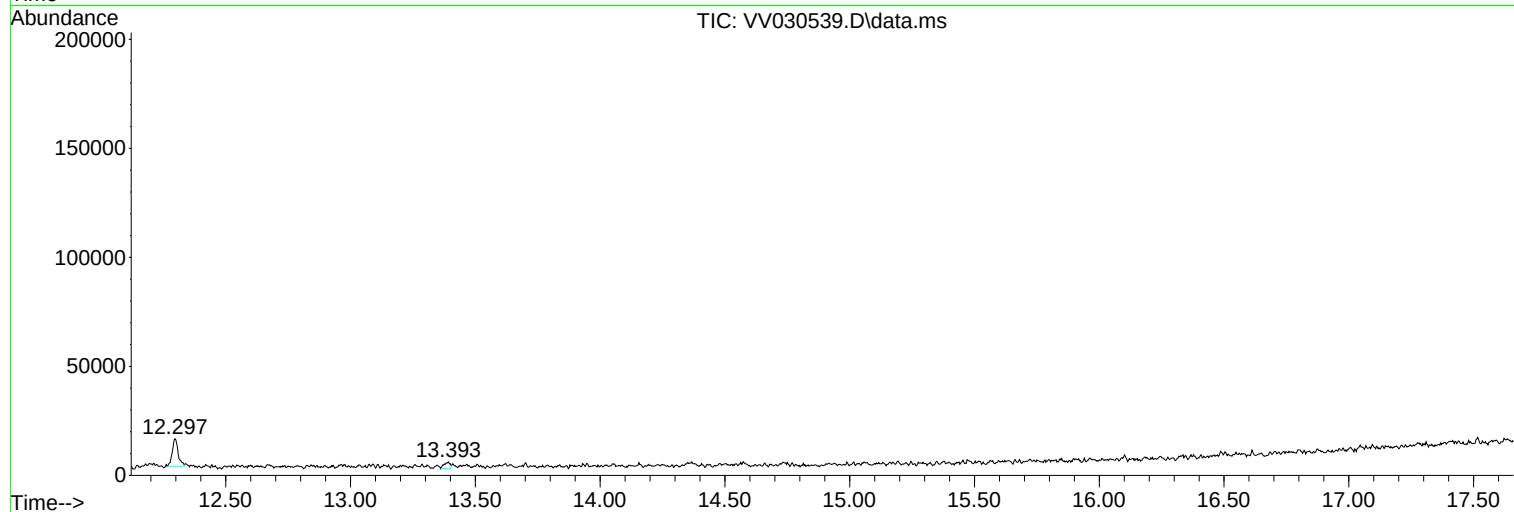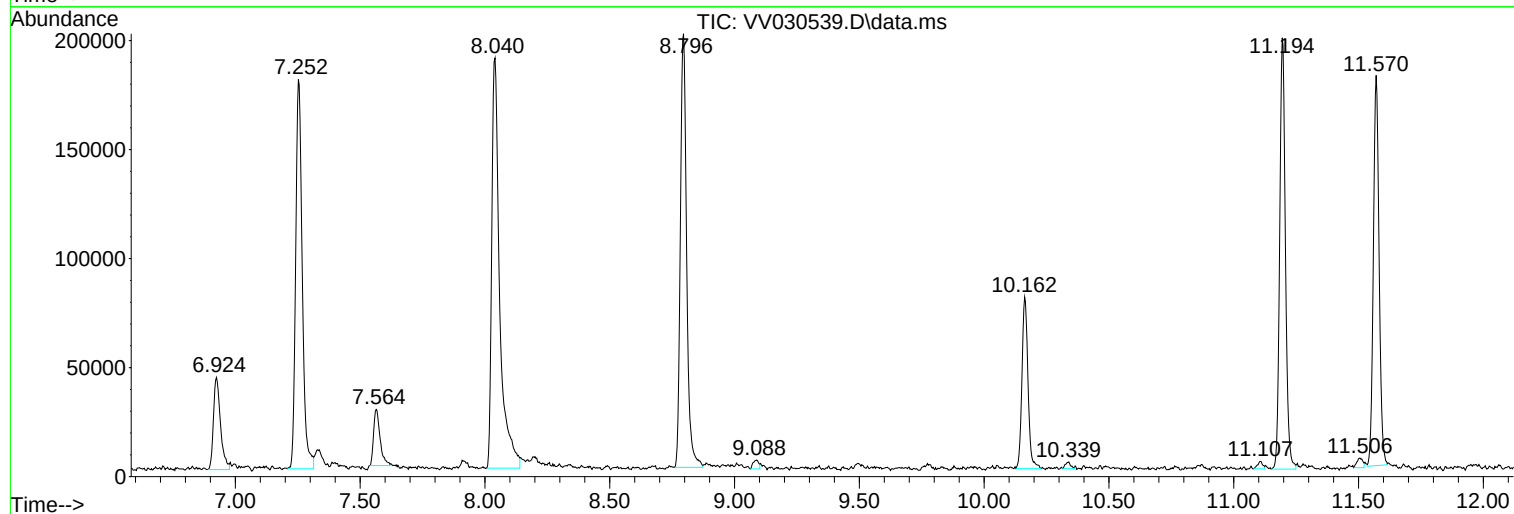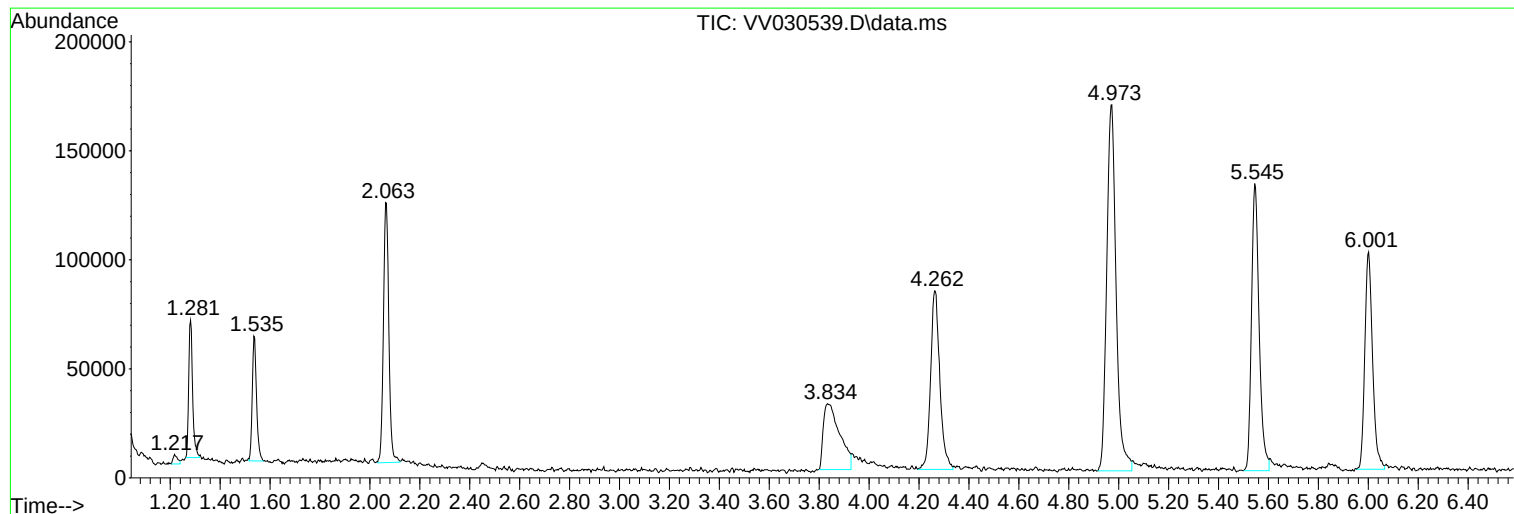

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030539.D
Acq On : 13 Apr 2023 12:46
Operator : SY/MD
Sample : 02254-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030539.D
Acq On : 13 Apr 2023 12:46
Operator : SY/MD
Sample : 02254-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
