

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
 Data File : VV030542.D
 Acq On : 13 Apr 2023 13:54
 Operator : SY/MD
 Sample : 02250-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDY5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030542.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	88	rBV	71102	76540	18.02%	2.031%
2	1.539	147	155	174	rVB	60440	77876	18.34%	2.066%
3	2.066	308	319	333	rBV	124449	183217	43.14%	4.861%
4	3.812	849	862	888	rBV	48716	159529	37.57%	4.233%
5	4.265	986	1003	1025	rBV2	83079	222024	52.28%	5.891%
6	4.969	1206	1222	1246	rBV3	160617	424659	100.00%	11.267%
7	5.545	1390	1401	1419	rBV	149866	310756	73.18%	8.245%
8	6.002	1529	1543	1561	rBV	100393	211414	49.78%	5.609%
9	6.924	1817	1830	1856	rBV	44822	94035	22.14%	2.495%
10	7.252	1916	1932	1949	rBV	180075	331256	78.01%	8.789%
11	7.564	2019	2029	2042	rBV2	27182	49194	11.58%	1.305%
12	7.918	2129	2139	2149	rVB3	15994	27932	6.58%	0.741%
13	8.037	2164	2176	2206	rBV	187054	384433	90.53%	10.200%
14	8.191	2213	2224	2241	rVB4	17939	35593	8.38%	0.944%
15	8.792	2400	2411	2429	rBV	236746	397689	93.65%	10.552%
16	10.162	2826	2837	2854	rVB2	71630	120780	28.44%	3.205%
17	10.336	2883	2891	2902	rBV5	5811	9928	2.34%	0.263%
18	11.194	3147	3158	3176	rBV	222055	357245	84.13%	9.479%
19	11.570	3263	3275	3293	rVB	178418	285365	67.20%	7.571%
20	12.294	3494	3500	3508	rBV9	6316	9531	2.24%	0.253%




Sum of corrected areas: 3768996

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030542.D
Acq On : 13 Apr 2023 13:54
Operator : SY/MD
Sample : 02250-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

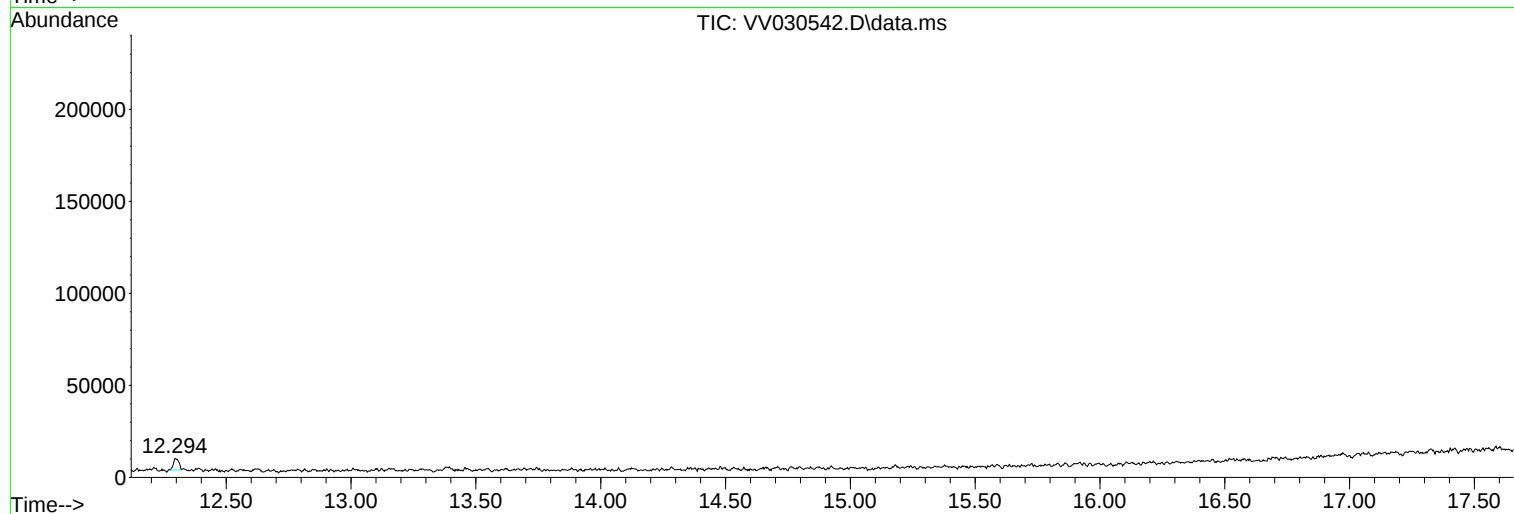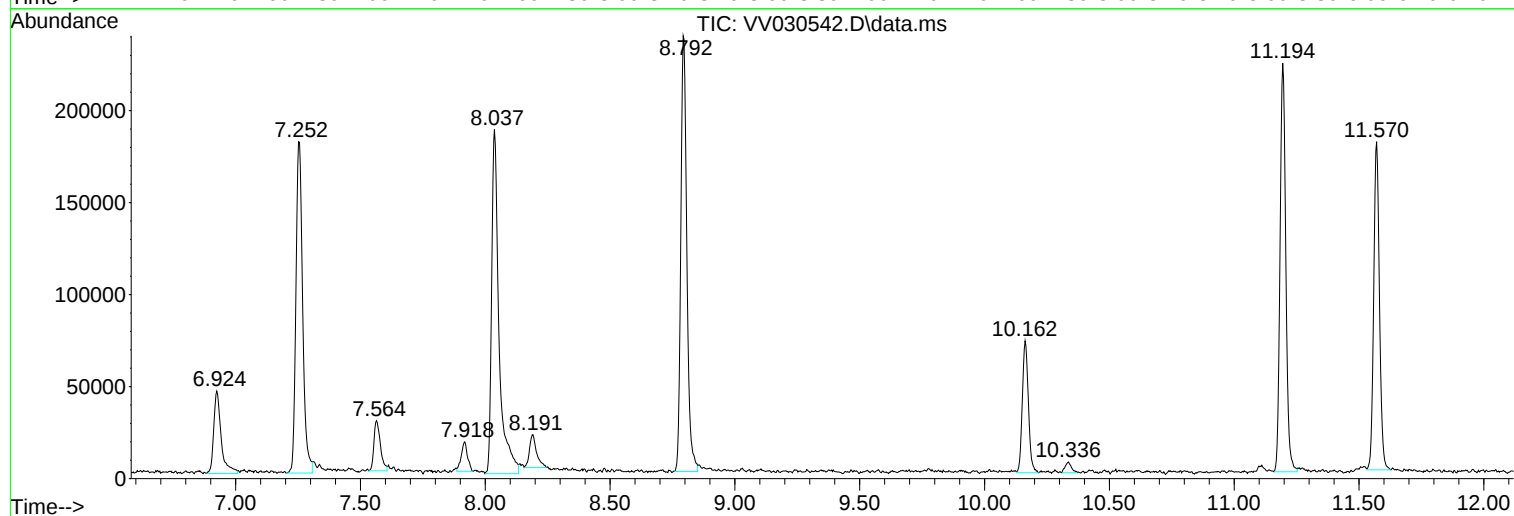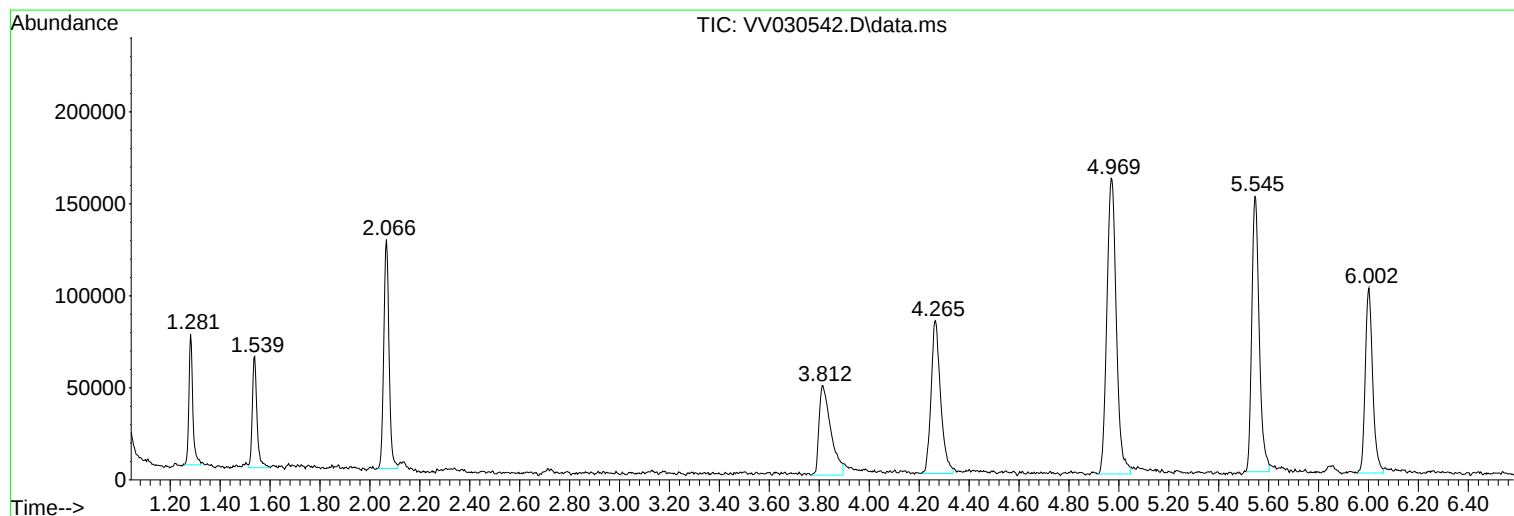

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030542.D
Acq On : 13 Apr 2023 13:54
Operator : SY/MD
Sample : 02250-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030542.D
Acq On : 13 Apr 2023 13:54
Operator : SY/MD
Sample : 02250-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------