

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
 Data File : VV030543.D
 Acq On : 13 Apr 2023 14:19
 Operator : SY/MD
 Sample : 02254-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030543.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	66	75	87	rBV	65693	77106	17.42%	2.157%
2	1.535	148	154	164	rBV	57827	67073	15.15%	1.876%
3	2.063	307	318	331	rBV	127937	189819	42.89%	5.310%
4	3.841	858	871	882	rBV	28334	95633	21.61%	2.675%
5	4.262	984	1002	1025	rBV	77577	209498	47.33%	5.860%
6	4.969	1204	1222	1254	rBV2	165570	442622	100.00%	12.381%
7	5.545	1385	1401	1424	rBV	136359	287916	65.05%	8.054%
8	6.001	1530	1543	1558	rBV2	98388	207424	46.86%	5.802%
9	6.924	1816	1830	1845	rBV2	44896	86443	19.53%	2.418%
10	7.252	1920	1932	1951	rBV	181018	333365	75.32%	9.325%
11	7.329	1954	1956	1964	rVB6	5067	5147	1.16%	0.144%
12	7.564	2020	2029	2051	rBV2	27339	51513	11.64%	1.441%
13	8.037	2165	2176	2202	rBV	174156	380505	85.97%	10.643%
14	8.792	2400	2411	2431	rBV	205010	351117	79.33%	9.821%
15	10.162	2826	2837	2854	rVB	74599	122305	27.63%	3.421%
16	10.329	2881	2889	2891	rBV8	4910	5203	1.18%	0.146%
17	11.101	3123	3129	3135	rBV8	3965	6088	1.38%	0.170%
18	11.194	3147	3158	3177	rBV	202593	325242	73.48%	9.098%
19	11.500	3241	3253	3263	rBV2	9785	20770	4.69%	0.581%
20	11.570	3263	3275	3291	rVB	180374	290029	65.53%	8.113%
21	12.297	3493	3501	3510	rBV6	13545	20206	4.57%	0.565%




Sum of corrected areas: 3575024

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030543.D
Acq On : 13 Apr 2023 14:19
Operator : SY/MD
Sample : 02254-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

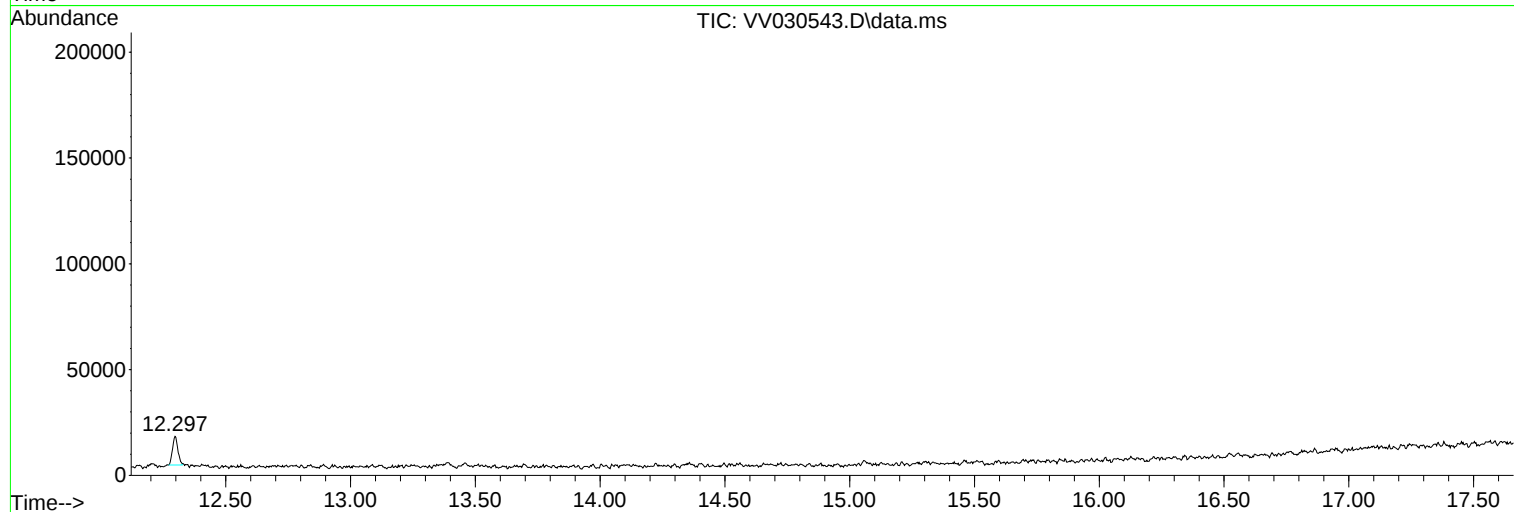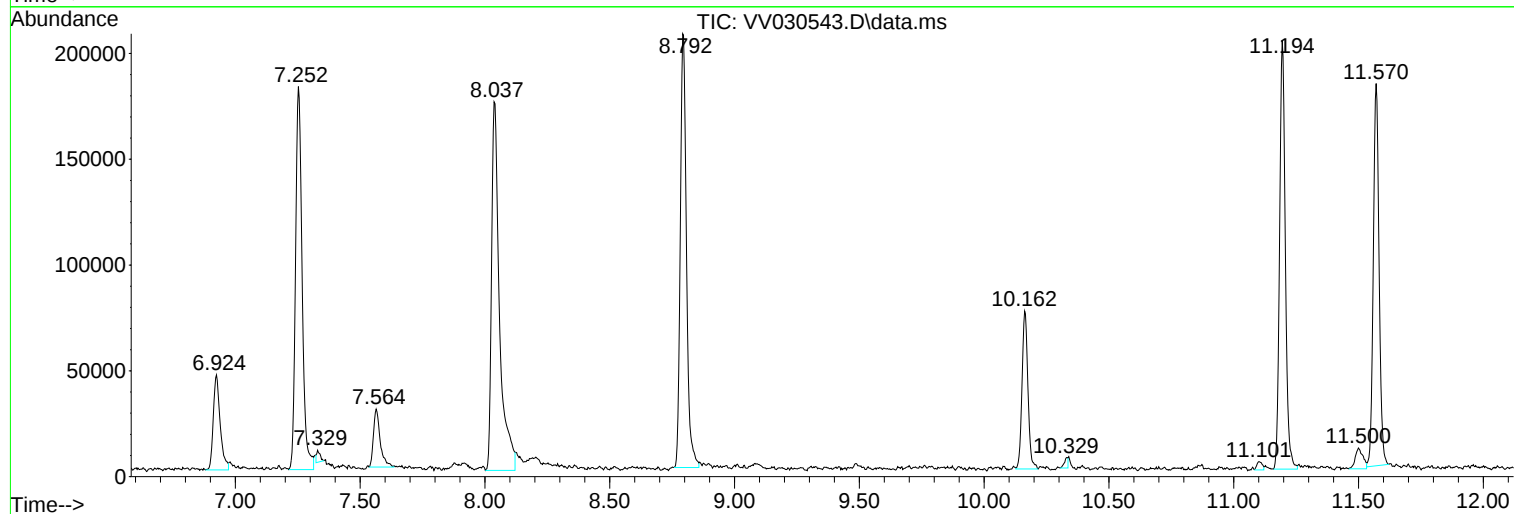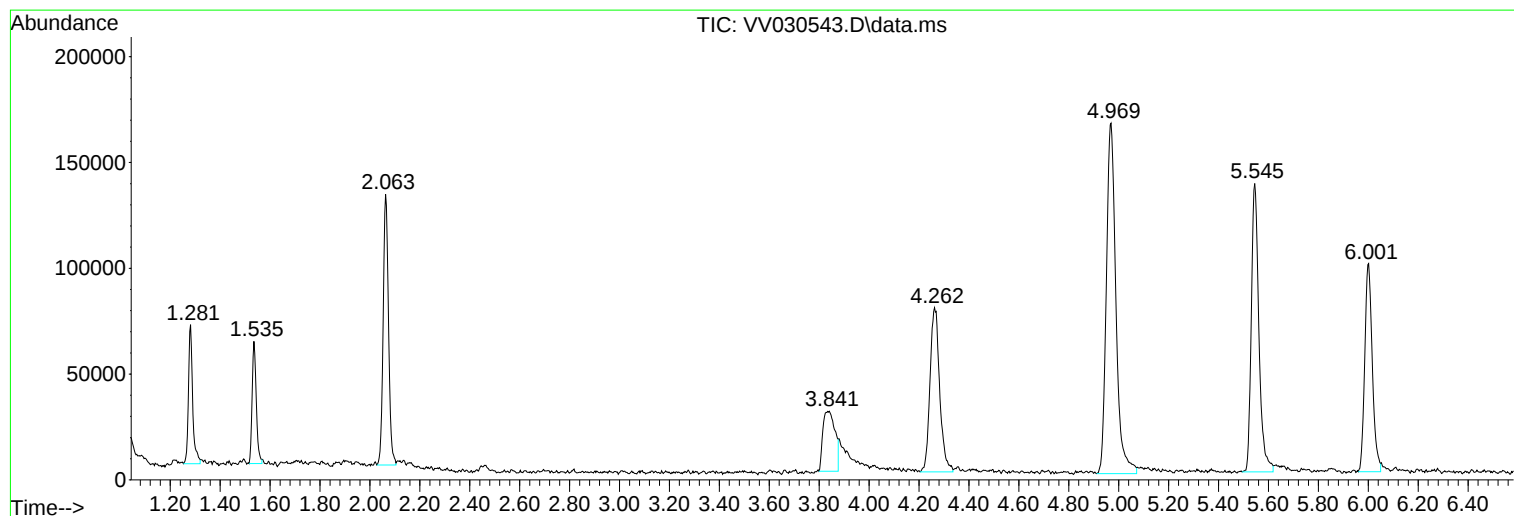

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030543.D
Acq On : 13 Apr 2023 14:19
Operator : SY/MD
Sample : 02254-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030543.D
Acq On : 13 Apr 2023 14:19
Operator : SY/MD
Sample : 02254-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------