

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
 Data File : VV030544.D
 Acq On : 13 Apr 2023 14:43
 Operator : SY/MD
 Sample : 02275-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDY7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030544.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	66	75	86	rBV	52715	60188	14.43%	2.006%
2	1.536	147	154	163	rBV	44984	51686	12.39%	1.723%
3	2.066	309	319	330	rBV	97404	140398	33.66%	4.680%
4	3.809	852	861	892	rBV	50482	157449	37.75%	5.248%
5	4.262	980	1002	1027	rBV2	59110	163294	39.15%	5.443%
6	4.966	1204	1221	1244	rBV2	128140	342656	82.15%	11.421%
7	5.545	1388	1401	1415	rBV	100275	210227	50.40%	7.007%
8	5.998	1529	1542	1561	rBV	76807	162329	38.92%	5.410%
9	6.924	1818	1830	1851	rBV2	33723	70272	16.85%	2.342%
10	7.252	1921	1932	1947	rBV	135905	243600	58.40%	8.119%
11	7.326	1948	1955	1967	rVB	21334	39754	9.53%	1.325%
12	7.564	2019	2029	2043	rBV2	22771	45426	10.89%	1.514%
13	7.912	2130	2137	2146	rVB2	5887	9555	2.29%	0.318%
14	8.037	2165	2176	2206	rBV	202561	417095	100.00%	13.902%
15	8.796	2397	2412	2433	rBV	155018	265300	63.61%	8.843%
16	10.162	2823	2837	2853	rBV2	74149	119157	28.57%	3.972%
17	10.333	2880	2890	2901	rVB3	9312	16472	3.95%	0.549%
18	11.194	3146	3158	3176	rBV	148927	242023	58.03%	8.067%
19	11.506	3248	3255	3263	rBV10	2837	5321	1.28%	0.177%
20	11.571	3264	3275	3288	rVV	139535	221417	53.09%	7.380%
21	12.297	3493	3501	3510	rBV9	10574	16641	3.99%	0.555%




Sum of corrected areas: 3000260

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030544.D
Acq On : 13 Apr 2023 14:43
Operator : SY/MD
Sample : 02275-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

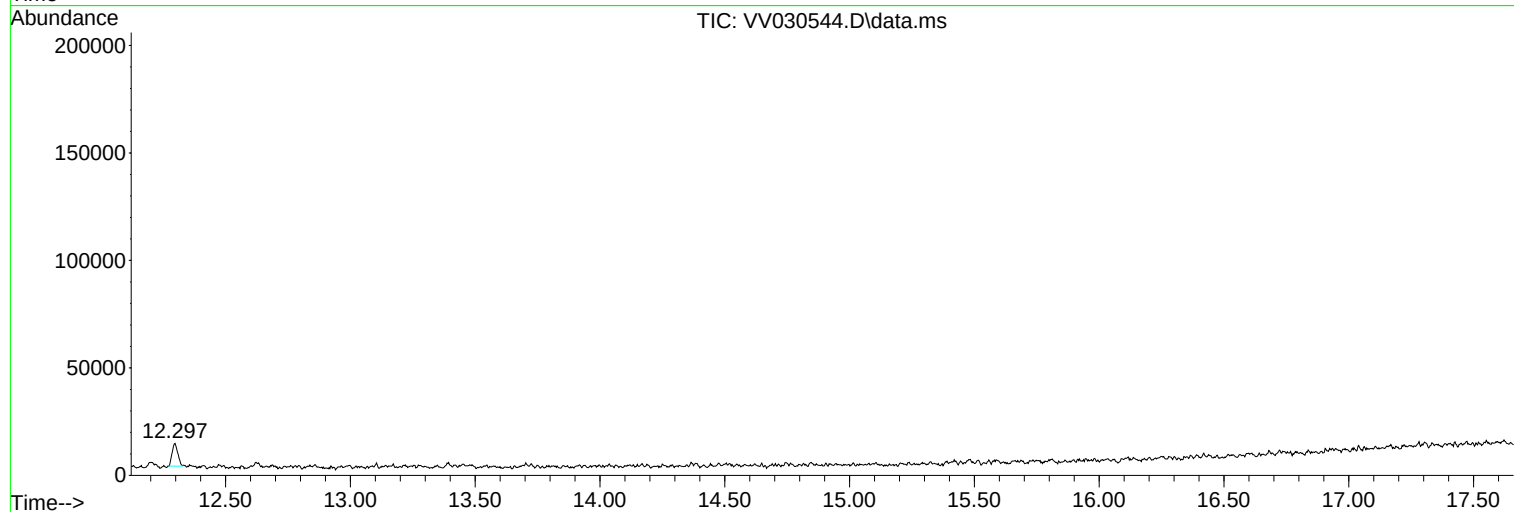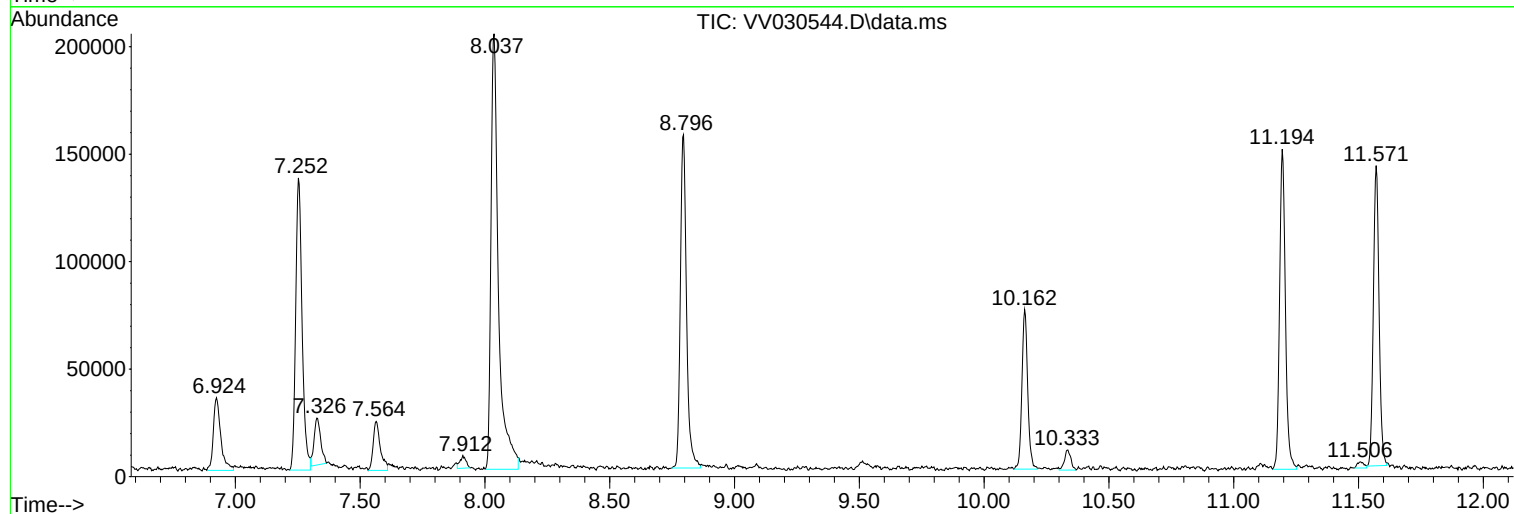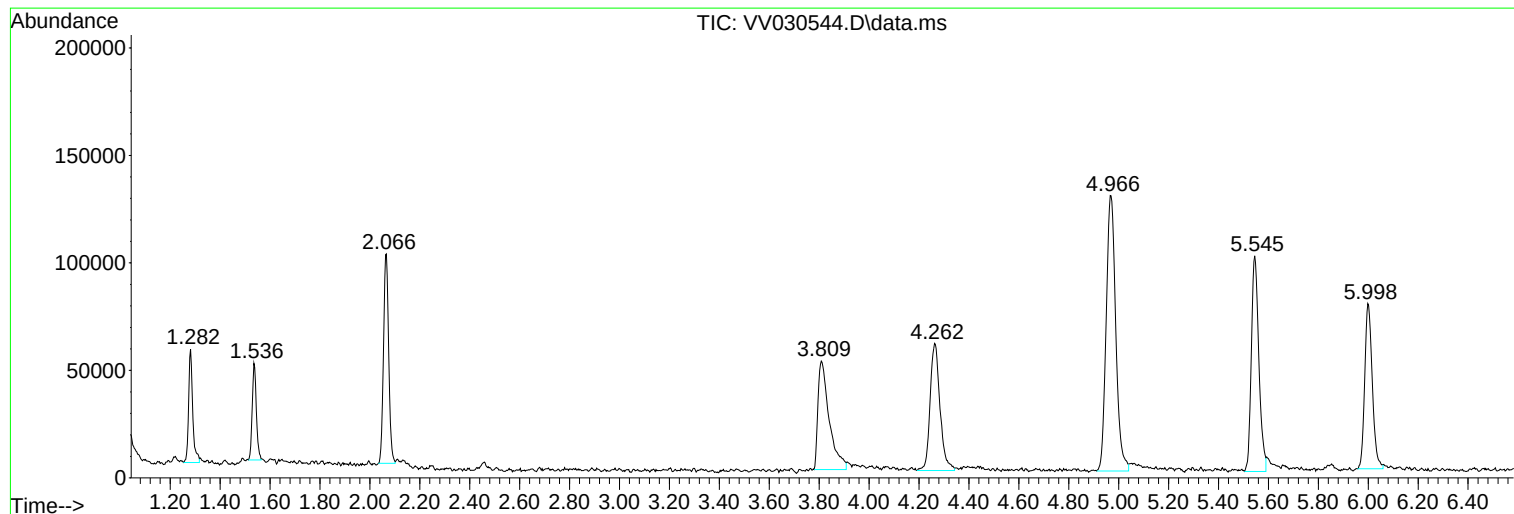

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030544.D
Acq On : 13 Apr 2023 14:43
Operator : SY/MD
Sample : 02275-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030544.D
Acq On : 13 Apr 2023 14:43
Operator : SY/MD
Sample : 02275-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------