

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
 Data File : VV030545.D
 Acq On : 13 Apr 2023 15:08
 Operator : SY/MD
 Sample : 02250-05DL 25X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHD6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	66	75	84	rBV	46258	52592	6.55%	1.004%
2	1.535	147	154	162	rBV	50280	58253	7.25%	1.112%
3	2.072	309	321	338	rBV3	401468	634701	79.05%	12.113%
4	3.124	632	648	670	rBV2	61838	134316	16.73%	2.563%
5	3.831	856	868	893	rBV2	45075	165176	20.57%	3.152%
6	4.262	987	1002	1024	rBV	76948	202087	25.17%	3.857%
7	4.526	1064	1084	1098	rBV2	18519	51634	6.43%	0.985%
8	4.969	1206	1222	1242	rBV2	161142	411781	51.28%	7.859%
9	5.545	1387	1401	1422	rBV	149515	321798	40.08%	6.142%
10	5.841	1480	1493	1515	rBV	404723	802960	100.00%	15.325%
11	5.998	1529	1542	1564	rVB	101082	209796	26.13%	4.004%
12	6.921	1816	1829	1846	rBV	41940	84846	10.57%	1.619%
13	7.252	1919	1932	1949	rBV	180534	327913	40.84%	6.258%
14	7.564	2020	2029	2038	rBV2	25633	45345	5.65%	0.865%
15	7.915	2120	2138	2158	rBV2	102224	184245	22.95%	3.516%
16	8.037	2164	2176	2206	rBV	178298	378186	47.10%	7.218%
17	8.792	2397	2411	2429	rBV	229895	399021	49.69%	7.615%
18	10.162	2826	2837	2849	rBV	73058	121822	15.17%	2.325%
19	11.194	3147	3158	3176	rBV	229293	363931	45.32%	6.946%
20	11.570	3261	3275	3289	rBV	179770	289220	36.02%	5.520%




Sum of corrected areas: 5239623

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030545.D
Acq On : 13 Apr 2023 15:08
Operator : SY/MD
Sample : 02250-05DL 25X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHD6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

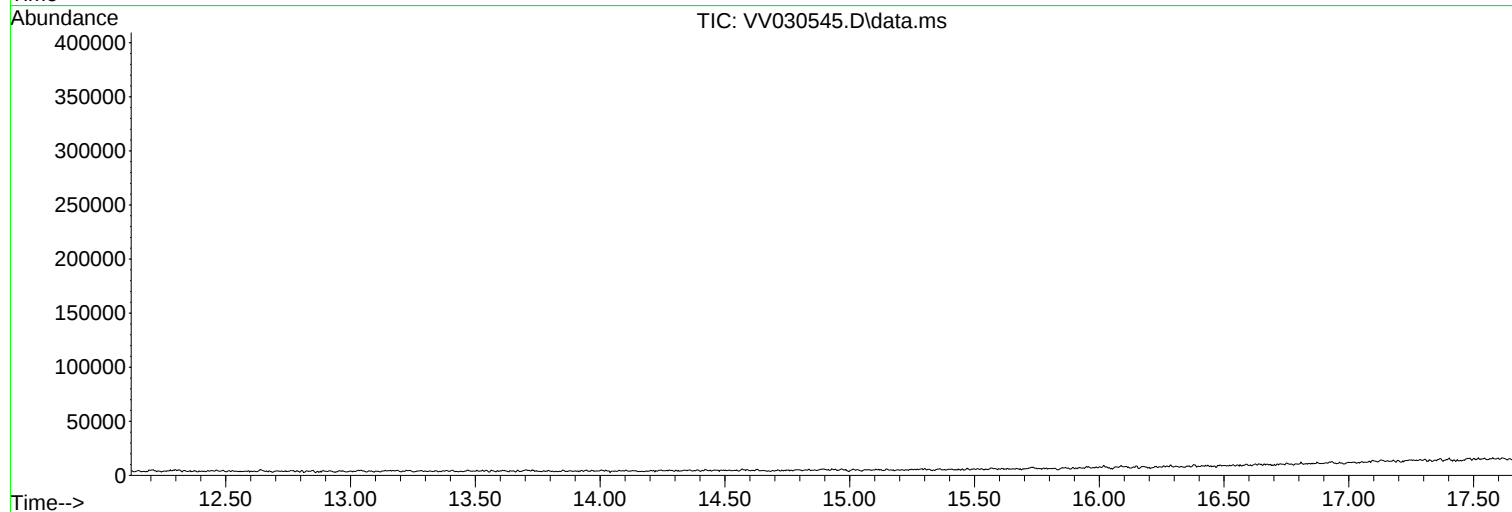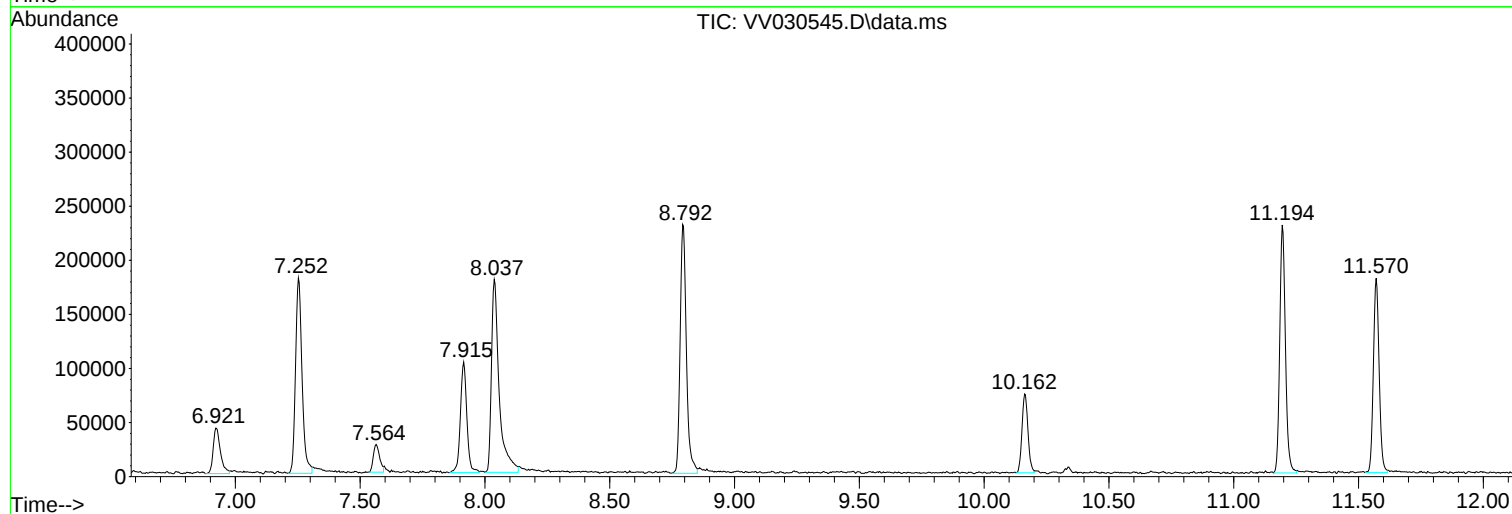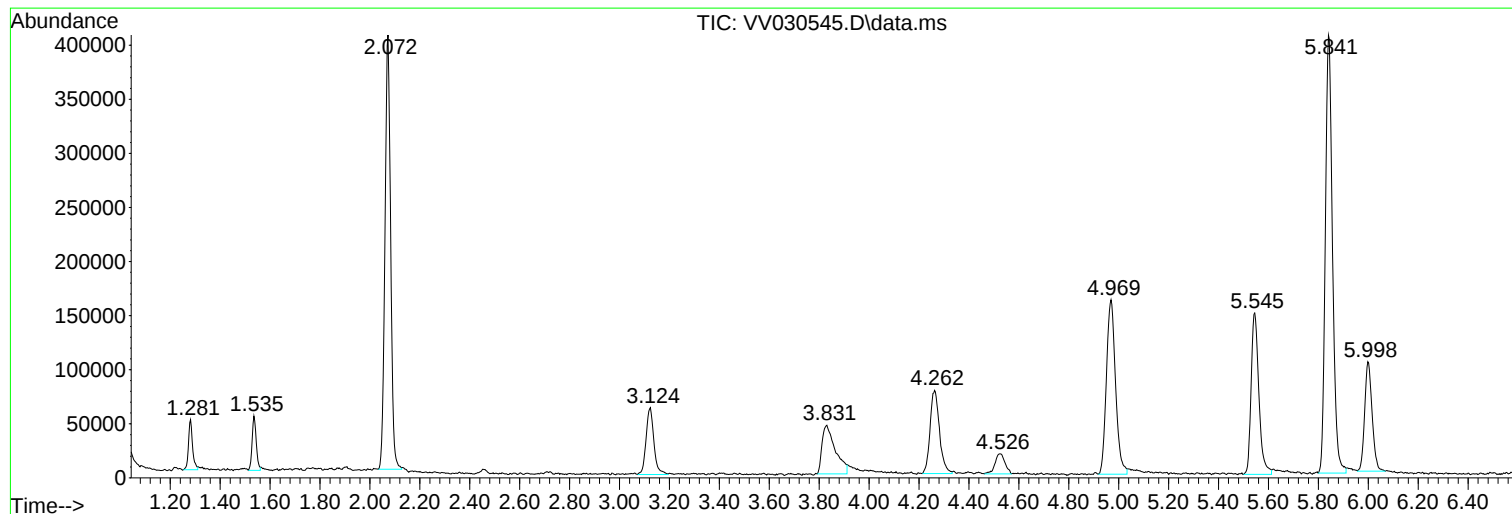

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030545.D
Acq On : 13 Apr 2023 15:08
Operator : SY/MD
Sample : 02250-05DL 25X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030545.D
Acq On : 13 Apr 2023 15:08
Operator : SY/MD
Sample : 02250-05DL 25X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------