


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041323\
Data File : VV030532.D
Acq On : 13 Apr 2023 09:22
Operator : SY/MD
Sample : BFB248
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB248

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Apr 14 05:16:37 2023

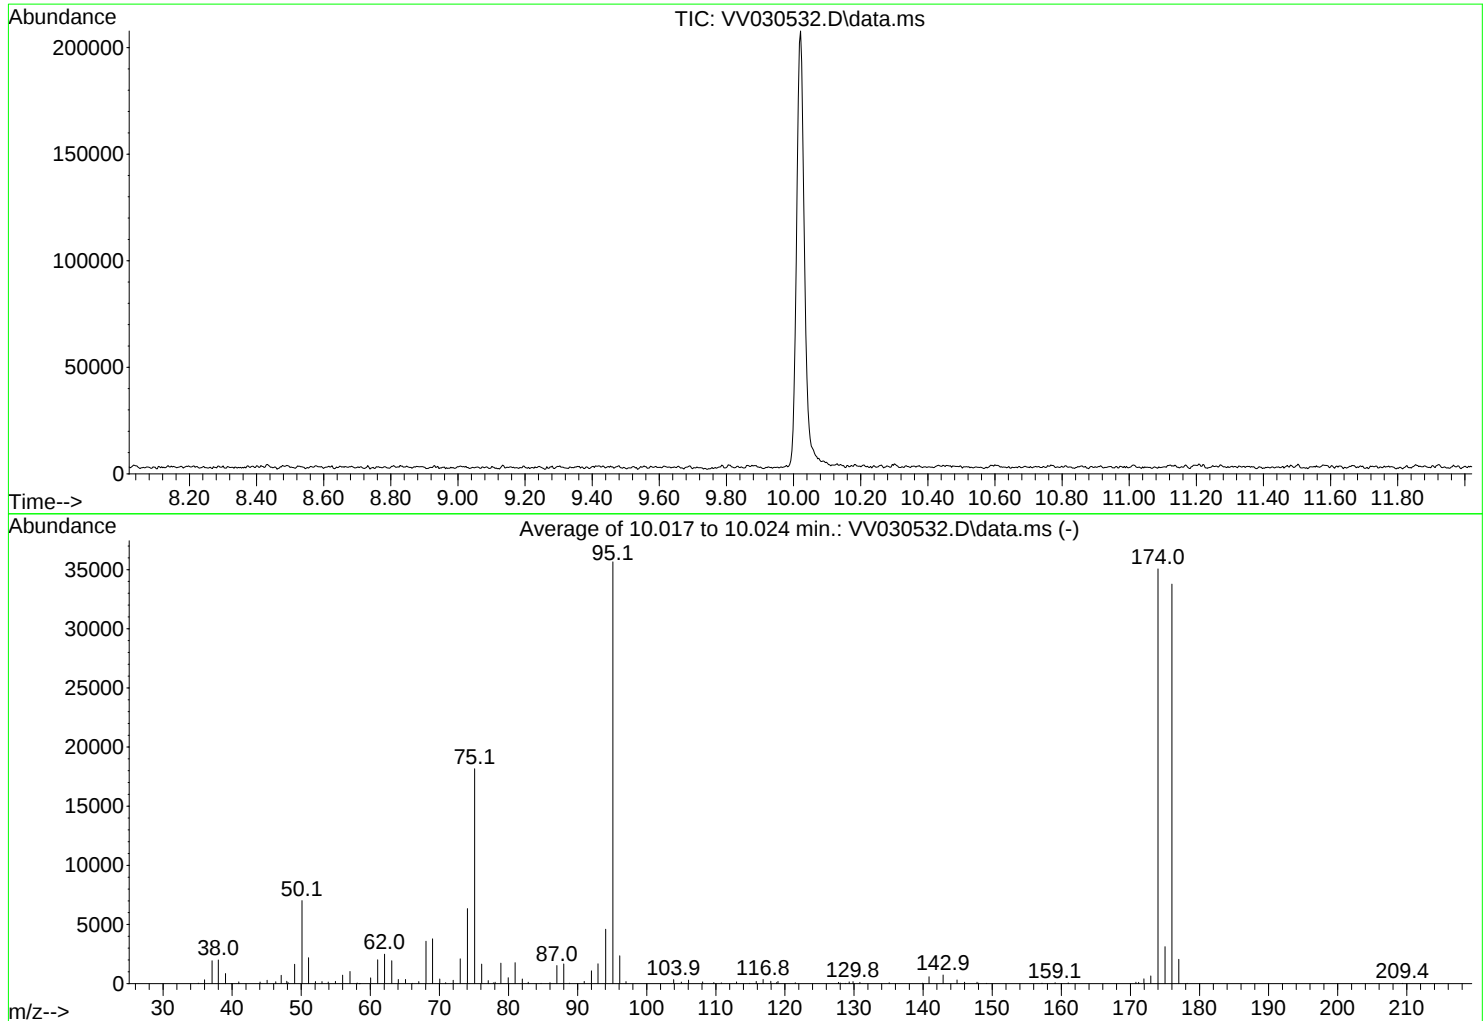

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2779

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	7027	PASS
75	95	30	80	50.9	18165	PASS
95	95	100	100	100.0	35659	PASS
96	95	5	9	6.6	2349	PASS
173	174	0.00	2	1.8	646	PASS
174	95	50	120	98.3	35064	PASS
175	174	5	9	8.9	3123	PASS
176	174	95	105	96.3	33781	PASS
177	176	5	10	6.1	2050	PASS

m/z	Abundance
35.40	122.0
36.00	200.0
36.90	100.0
37.70	117.0
38.30	133.0
38.90	114.0
39.80	228.0
40.30	250.0
41.80	123.0
43.20	166.0
44.00	294.0
45.10	153.0
49.00	114.0
49.50	102.0
50.20	120.0
55.50	105.0
56.80	119.0
57.30	140.0
58.40	131.0
62.80	122.0
63.50	107.0
64.20	109.0
69.00	134.0
85.50	101.0
92.80	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB248

m/z	Abundance
35.10	139.0
36.00	562.0
37.10	1990.0
38.00	2139.0
39.10	1040.0
39.90	205.0
40.90	133.0
43.00	126.0
44.20	453.0
45.00	417.0
46.30	144.0
47.10	625.0
47.90	296.0
49.10	1827.0
50.10	7235.0
51.10	2336.0
52.10	181.0
53.00	155.0
53.90	116.0
54.90	208.0
56.00	692.0
57.10	1036.0
58.10	143.0
58.50	135.0
60.10	518.0
61.00	1896.0
62.00	2575.0
63.10	1982.0
64.00	514.0
65.10	358.0
67.00	158.0
68.10	3658.0
69.00	4095.0
70.00	477.0
72.00	306.0
73.00	2035.0
74.00	6340.0
75.10	18600.0
76.10	1676.0
77.10	246.0
77.80	203.0
78.90	1790.0
79.90	471.0
80.90	1844.0
82.00	391.0
82.80	130.0
84.70	103.0
86.00	114.0
87.00	1487.0
88.00	1488.0
88.80	109.0
91.00	220.0
92.00	1114.0
93.00	1756.0
94.00	4466.0
95.10	36104.0
96.10	2522.0
97.00	200.0
103.90	327.0
104.90	112.0
106.00	303.0
108.10	106.0
109.70	151.0
113.00	144.0
115.80	187.0
116.80	357.0
117.90	190.0
118.80	298.0
121.50	115.0
127.70	171.0
129.20	149.0
129.90	187.0
130.90	104.0
139.90	110.0
140.80	570.0
142.90	726.0
144.90	291.0
146.00	128.0
147.80	190.0
161.00	102.0
170.90	120.0
171.90	378.0
172.90	570.0
174.00	34280.0
175.00	3142.0
176.00	34056.0
177.00	2065.0
178.20	100.0
209.40	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB248

m/z	Abundance
36.00	541.0
37.10	1980.0
38.00	2136.0
39.10	1000.0
40.00	228.0
41.00	160.0
43.00	138.0
44.10	443.0
45.10	447.0
46.30	182.0
47.10	756.0
47.90	324.0
49.10	1793.0
50.10	7342.0
51.10	2266.0
52.00	174.0
53.00	188.0
53.90	141.0
55.00	192.0
56.00	753.0
57.10	1048.0
58.40	133.0
60.00	494.0
61.00	2086.0
62.10	2587.0
63.10	2017.0
64.00	476.0
65.10	368.0
67.00	173.0
68.00	3652.0
69.00	4039.0
70.00	396.0
70.90	114.0
72.00	302.0
73.00	2221.0
74.10	6531.0
75.10	18824.0
76.10	1678.0
77.00	253.0
78.10	185.0
78.90	1796.0
80.00	499.0
80.90	1826.0
82.00	409.0
82.80	129.0
86.00	118.0
87.00	1582.0
88.00	1723.0
90.90	184.0
92.00	1120.0
93.00	1812.0
94.10	4777.0
95.10	36936.0
96.10	2445.0
97.00	186.0
103.90	351.0
105.00	141.0
106.00	324.0
108.10	164.0
109.70	142.0
110.80	101.0
113.00	157.0
114.90	102.0
115.90	198.0
116.90	372.0
118.00	206.0
119.00	288.0
121.50	113.0
127.80	156.0
129.30	166.0
129.90	179.0
130.80	114.0
135.10	127.0
140.90	588.0
142.90	753.0
144.90	316.0
146.00	119.0
147.80	163.0
149.20	102.0
159.10	125.0
161.00	100.0
170.80	128.0
171.20	139.0
171.90	413.0
173.00	653.0
174.00	36264.0
175.00	3201.0
176.00	34856.0
177.00	2149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB248

m/z	Abundance
36.00	491.0
37.10	1825.0
38.00	1746.0
39.10	855.0
40.10	255.0
41.00	160.0
43.00	137.0
44.10	396.0
45.10	442.0
46.30	153.0
47.10	748.0
48.10	281.0
49.10	1626.0
50.10	6863.0
51.00	1992.0
52.00	163.0
53.00	201.0
53.90	144.0
55.00	169.0
56.00	701.0
57.00	991.0
58.30	135.0
60.00	470.0
61.10	2077.0
62.10	2318.0
63.10	1807.0
64.10	396.0
65.10	345.0
66.10	101.0
67.00	207.0
68.00	3435.0
69.00	3620.0
70.10	300.0
70.90	134.0
72.00	261.0
73.00	2019.0
74.10	6149.0
75.10	17072.0
76.10	1611.0
77.00	274.0
78.00	187.0
78.90	1614.0
80.00	518.0
81.00	1657.0
82.00	367.0
82.90	117.0
87.00	1509.0
88.00	1793.0
90.90	173.0
92.00	1026.0
93.00	1814.0
94.10	4567.0
95.10	33936.0
96.10	2079.0
97.00	147.0
103.90	322.0
105.10	140.0
106.10	286.0
108.10	166.0
110.80	113.0
113.00	136.0
115.90	204.0
116.80	339.0
117.90	214.0
119.00	298.0
128.00	151.0
128.80	105.0
129.40	135.0
129.80	179.0
130.80	104.0
135.10	115.0
140.90	581.0
142.90	698.0
144.90	320.0
146.00	107.0
148.00	112.0
157.20	114.0
159.10	138.0
170.70	126.0
171.20	170.0
172.00	448.0
173.00	715.0
174.00	34648.0
175.00	3026.0
176.00	32432.0
177.00	1935.0

Instrument :
MSVOA_V
ClientSampleId :
BFB248