

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041420\
 Data File : VV015471.D
 Acq On : 14 Apr 2020 19:12
 Operator : SY/MD
 Sample : L2273-13
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAQ91

Quant Time: Apr 15 05:04:29 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 15 02:17:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	116670	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	110034	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	53794	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	32499	5.37	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.40%
7) Chloroethane-d5	1.58	69	28663	5.14	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.80%
11) 1,1-Dichloroethene-d2	2.12	63	44807	3.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.20%
20) 2-Butanone-d5	3.95	46	80324	47.26	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.52%
24) Chloroform-d	4.38	84	60043	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.60%
26) 1,2-Dichloroethane-d4	5.06	65	34300	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.00%
32) Benzene-d6	5.08	84	120748	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
36) 1,2-Dichloropropane-d6	6.09	67	37287	4.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.00%
41) Toluene-d8	7.34	98	114340	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.20%
43) trans-1,3-Dichloropropene-	7.65	79	14953	4.52	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.40%
46) 2-Hexanone-d5	8.11	63	65418	41.02	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.04%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	26769	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.80%
64) 1,2-Dichlorobenzene-d4	11.65	152	41846	4.85	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.00%


Target Compounds					Ovalue
13) Acetone	2.23	43	8494	7.073 ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV041420\
Data File : VV015471.D
Acq On : 14 Apr 2020 19:12
Operator : SY/MD
Sample : L2273-13
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAQ91

Quant Time: Apr 15 05:04:29 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 15 02:17:02 2020
Response via : Initial Calibration

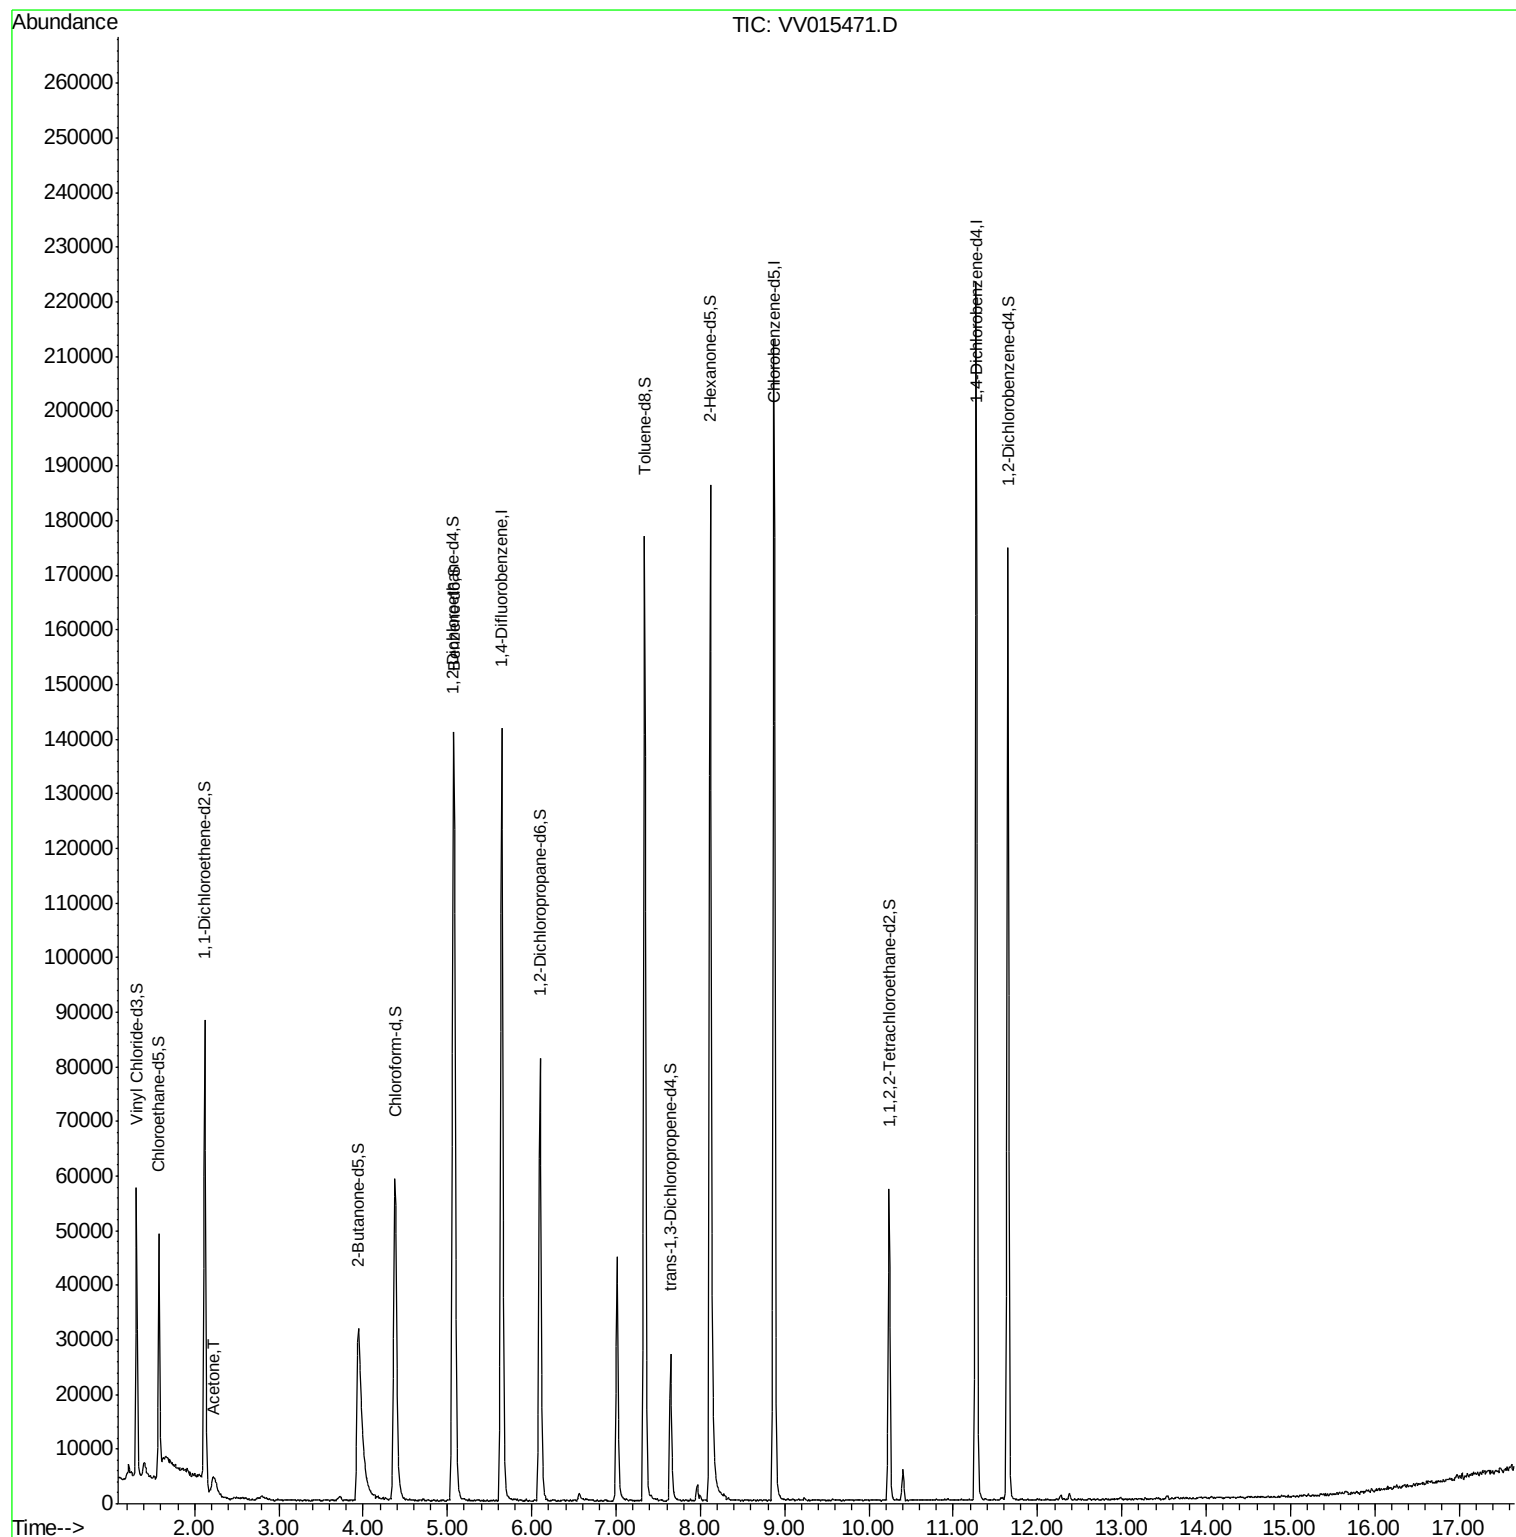

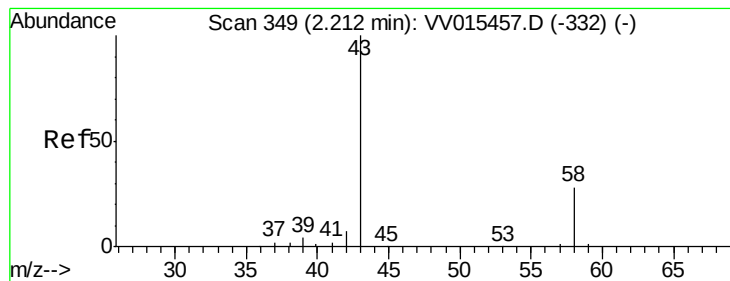

#13

Acetone

Concen: 7.073 ug/L

RT: 2.23 min Scan# 354

Delta R.T. 0.02 min

Lab File: VV015471.D

Acq: 14 Apr 2020 19:12

Instrument :
MSVOA_V
ClientSampleId :
YAQ91

Tot Ion: 43 Resp: 8494

Ion Ratio Lower Upper

43 100

58 23.0 0.0 22.2#

