

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041420\
 Data File : VV015473.D
 Acq On : 14 Apr 2020 19:59
 Operator : SY/MD
 Sample : L2273-15
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAQ93

Quant Time: Apr 15 05:10:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 15 02:17:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	118340	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	111013	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	55240	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	32422	5.28	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	105.60%
7) Chloroethane-d5	1.58	69	28343	5.01	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.20%
11) 1,1-Dichloroethene-d2	2.12	63	45740	3.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.80%
20) 2-Butanone-d5	3.92	46	75194	43.61	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.22%
24) Chloroform-d	4.38	84	60886	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.60%
26) 1,2-Dichloroethane-d4	5.06	65	33396	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.20%
32) Benzene-d6	5.08	84	120800	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
36) 1,2-Dichloropropane-d6	6.10	67	36965	4.82	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.40%
41) Toluene-d8	7.34	98	113799	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
43) trans-1,3-Dichloropropene-	7.65	79	14360	4.30	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.00%
46) 2-Hexanone-d5	8.11	63	61400	38.16	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.32%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	25308	4.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.20%
64) 1,2-Dichlorobenzene-d4	11.65	152	41605	4.69	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.80%


Target Compounds					Ovalue
13) Acetone	2.20	43	9095	7.467 ug/L	# 45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV041420\
Data File : VV015473.D
Acq On : 14 Apr 2020 19:59
Operator : SY/MD
Sample : L2273-15
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAQ93

Quant Time: Apr 15 05:10:47 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 15 02:17:02 2020
Response via : Initial Calibration

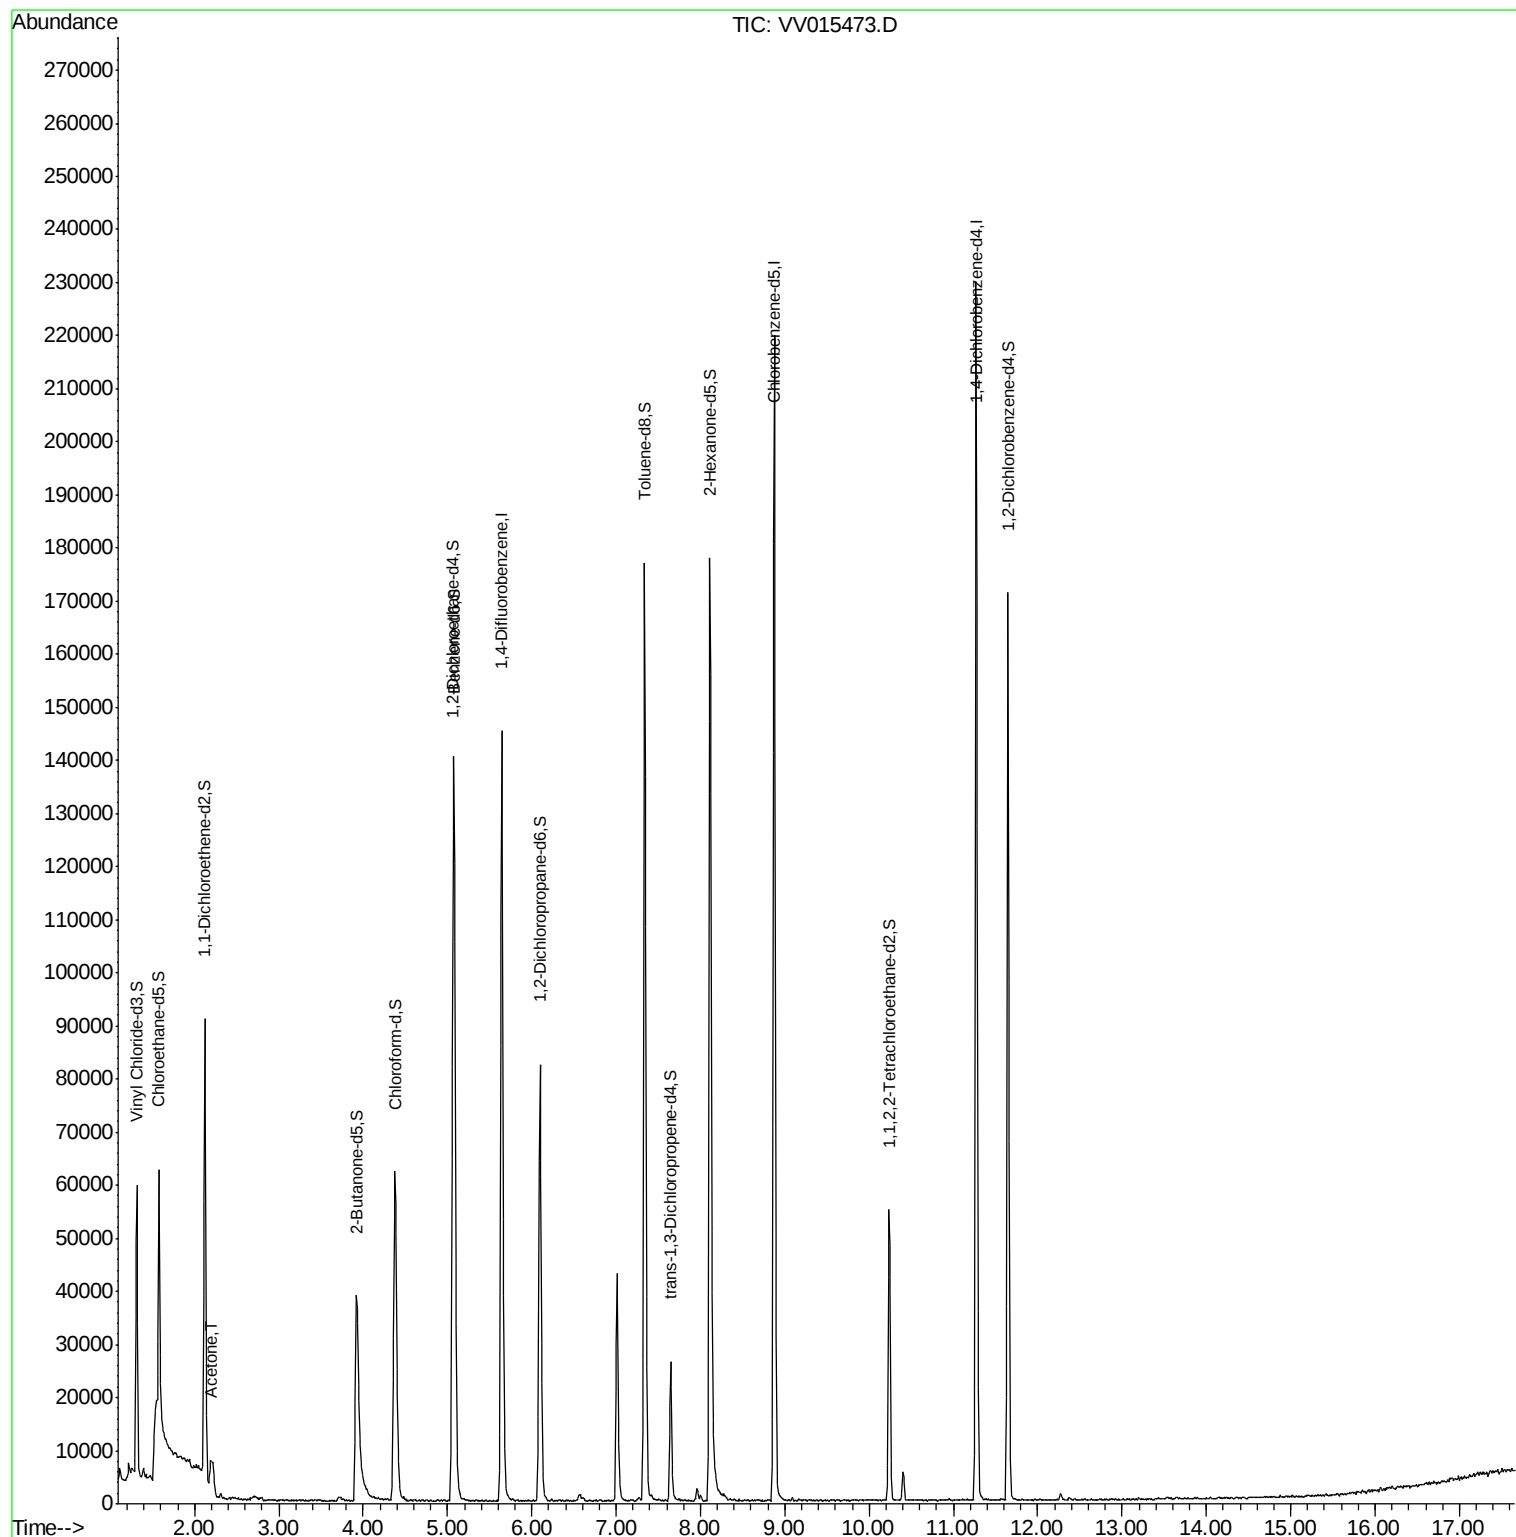

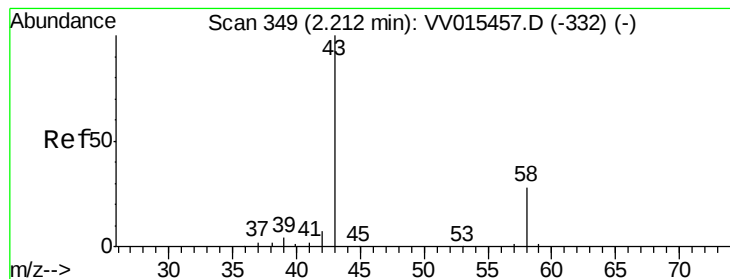

#13

Acetone

Concen: 7.467 ug/L

RT: 2.20 min Scan# 344

Delta R.T. -0.02 min

Lab File: VV015473.D

Acq: 14 Apr 2020 19:59

Instrument :
MSVOA_V
ClientSampleId :
YAQ93

Tot Ion: 43 Resp: 9095

Ion Ratio Lower Upper

43 100

58 31.8 0.0 22.2#

