

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041420\
 Data File : VV015488.D
 Acq On : 15 Apr 2020 02:11
 Operator : SY/MD
 Sample : L2274-08
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAQA6

Quant Time: Apr 15 06:32:32 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 15 05:31:01 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	109340	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	104568	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	50858	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	31248	5.51	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	110.20%
7) Chloroethane-d5	1.58	69	27778	5.32	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.40%
11) 1,1-Dichloroethene-d2	2.12	63	44727	3.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.80%
20) 2-Butanone-d5	3.93	46	78305	49.16	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.32%
24) Chloroform-d	4.38	84	63032	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.40%
26) 1,2-Dichloroethane-d4	5.06	65	33565	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.20%
32) Benzene-d6	5.08	84	119150	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.80%
36) 1,2-Dichloropropane-d6	6.10	67	36764	5.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.80%
41) Toluene-d8	7.34	98	109089	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.60%
43) trans-1,3-Dichloropropene-	7.65	79	13888	4.42	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.40%
46) 2-Hexanone-d5	8.11	63	64538	42.59	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.18%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	26316	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.80%
64) 1,2-Dichlorobenzene-d4	11.65	152	40821	5.00	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.00%

Target Compounds


					Ovalue
2) Dichlorodifluoromethane	1.14	85	6104	0.564 ug/L	95
13) Acetone	2.21	43	9933	8.826 ug/L #	57
25) Chloroform	4.41	83	176238	11.811 ug/L	99
47) Tetrachloroethene	8.00	164	308233	49.387 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV041420\
Data File : VV015488.D
Acq On : 15 Apr 2020 02:11
Operator : SY/MD
Sample : L2274-08
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAQA6

Quant Time: Apr 15 06:32:32 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 15 05:31:01 2020
Response via : Initial Calibration

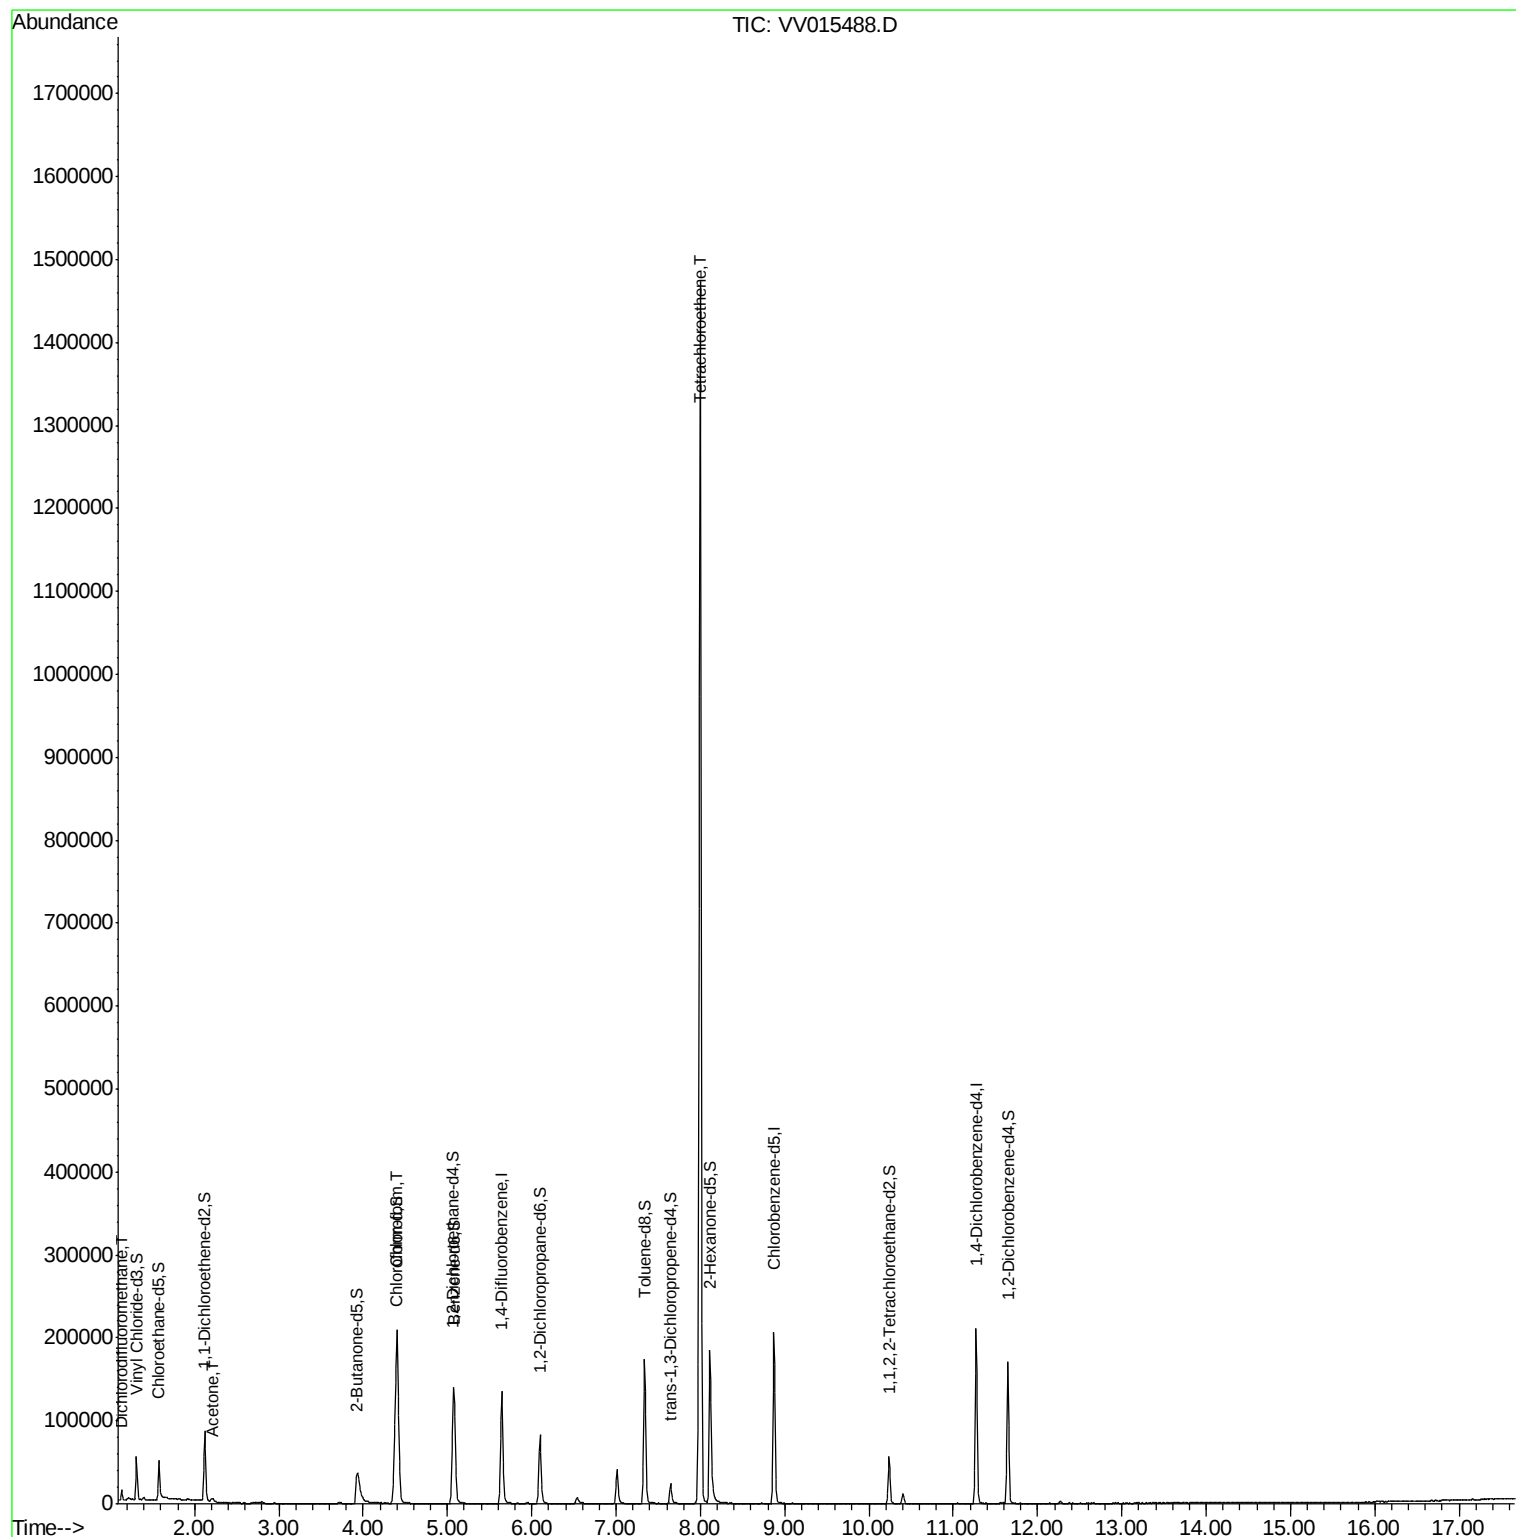

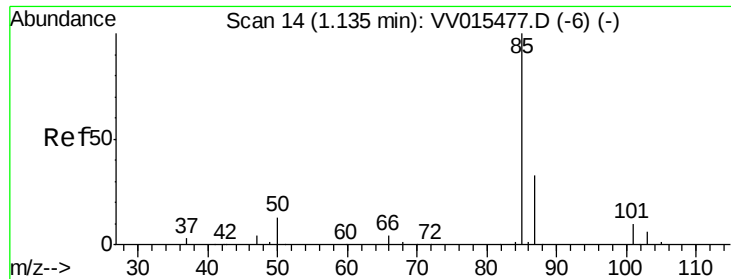

#2

Dichlorodifluoromethane

Concen: 0.564 ug/L

RT: 1.14 min Scan# 14

Delta R.T. 0.00 min

Lab File: VV015488.D

Acq: 15 Apr 2020 02:11

Instrument :

MSVOA_V

ClientSampleId :


YQA6

Tot Ion: 85 Resp: 6104

Ion Ratio Lower Upper




85 100

87 34.6 25.3 37.9

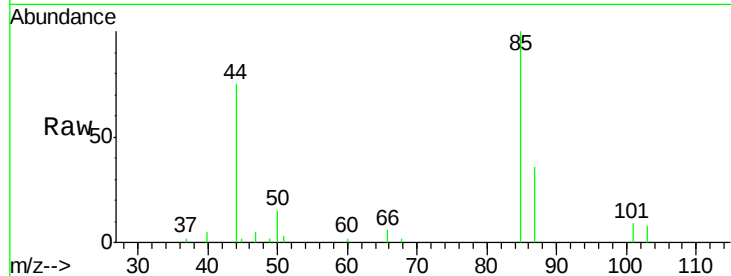

Abundance Ion 85.00 (84.70 to 85.70): VV0

Ion 87.00 (86.70 to 87.70): VV0

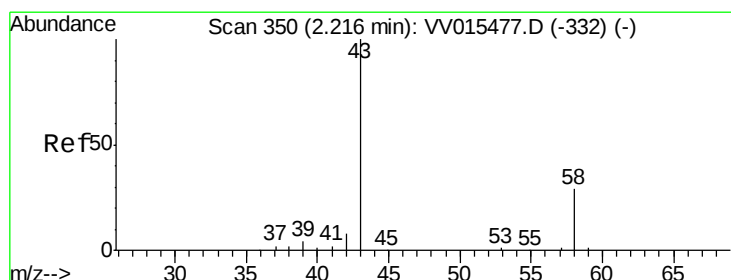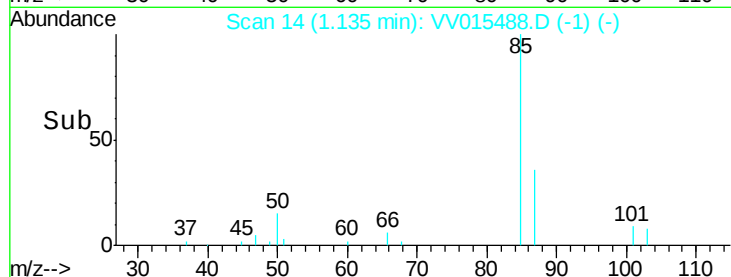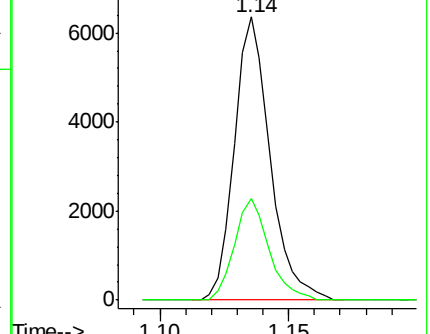

#13

Acetone

Concen: 8.826 ug/L

RT: 2.21 min Scan# 349

Delta R.T. -0.00 min

Lab File: VV015488.D


Acq: 15 Apr 2020 02:11

Tgt Ion: 43 Resp: 9933

Ion Ratio Lower Upper



43 100


58 27.5 0.0 22.2#

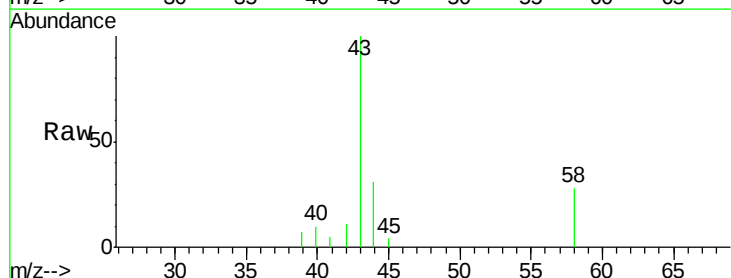

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0



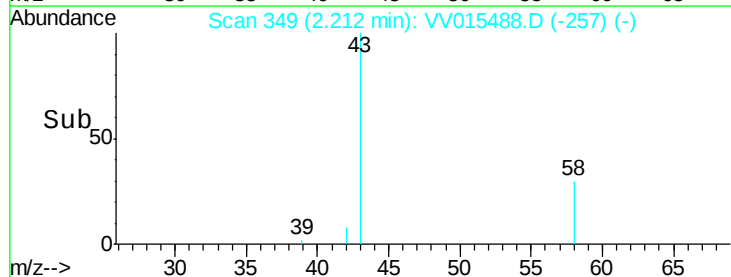
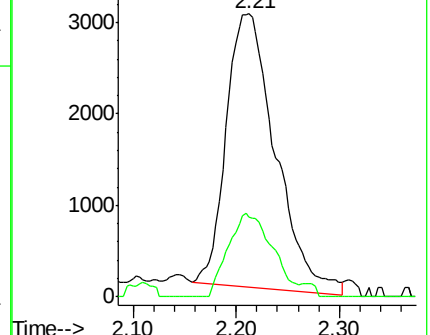


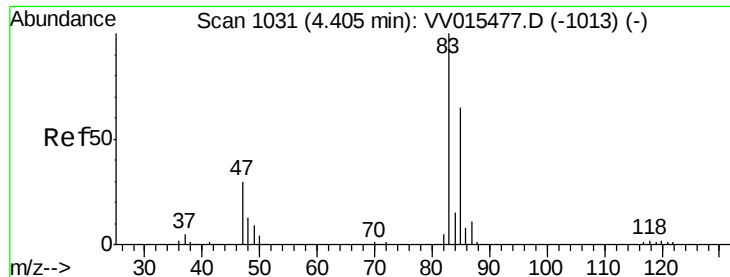

#25
Chloroform
Concen: 11.811 ug/L
RT: 4.41 min Scan# 1031
Delta R.T. 0.00 min
Lab File: VV015488.D
Acq: 15 Apr 2020 02:11

Instrument :
MSVOA_V
ClientSampleId :
YQA6

Tot Ion: 83 Resp: 176238
Ion Ratio Lower Upper
83 100
85 66.6 45.9 85.3

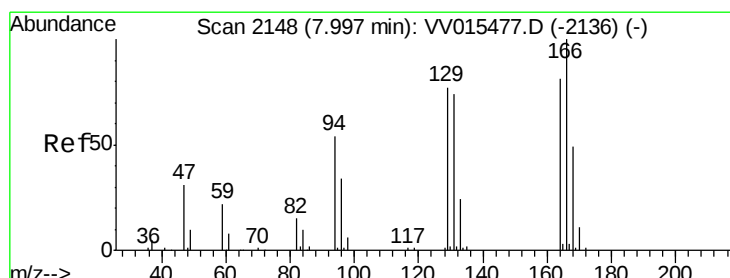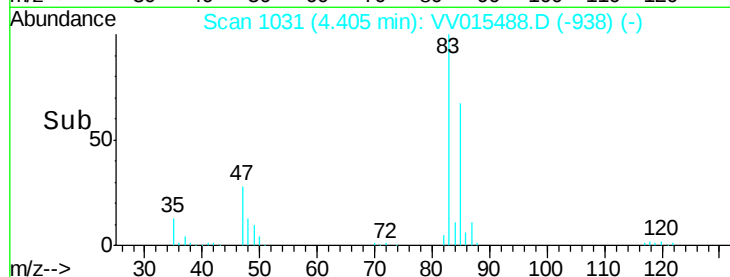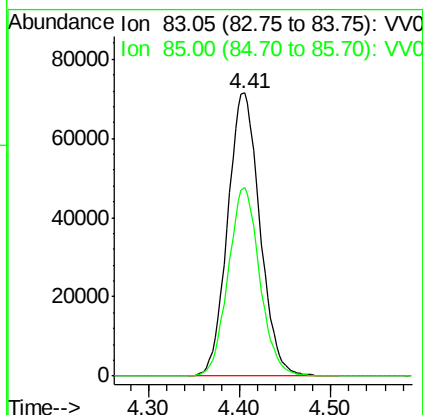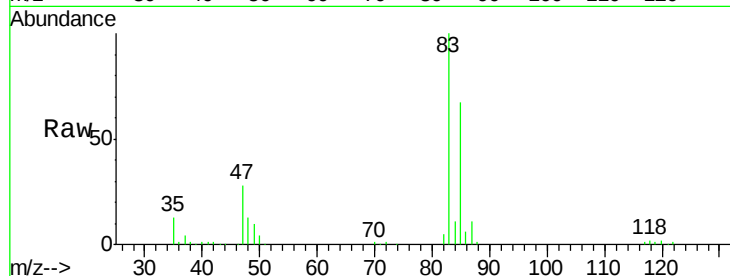

#47
Tetrachloroethene
Concen: 49.387 ug/L
RT: 8.00 min Scan# 2148
Delta R.T. 0.00 min
Lab File: VV015488.D
Acq: 15 Apr 2020 02:11

Tgt Ion: 164 Resp: 308233
Ion Ratio Lower Upper
164 100
129 98.3 70.6 131.0
131 94.2 68.3 126.8
166 126.8 88.3 163.9

