

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041420\
 Data File : VV015494.D
 Acq On : 15 Apr 2020 04:31
 Operator : SY/MD
 Sample : L2274-14
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YaqB2

Quant Time: Apr 15 07:07:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 15 05:31:01 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	106929	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	102090	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	50447	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	31128	5.61	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	112.20%
7) Chloroethane-d5	1.58	69	26826	5.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.00%
11) 1,1-Dichloroethene-d2	2.12	63	43709	3.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.80%
20) 2-Butanone-d5	3.92	46	75448	48.43	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.86%
24) Chloroform-d	4.38	84	54671	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.00%
26) 1,2-Dichloroethane-d4	5.06	65	32626	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.60%
32) Benzene-d6	5.08	84	118014	5.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.20%
36) 1,2-Dichloropropane-d6	6.10	67	35890	5.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.80%
41) Toluene-d8	7.34	98	109655	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.40%
43) trans-1,3-Dichloropropene-	7.65	79	13431	4.38	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.60%
46) 2-Hexanone-d5	8.11	63	61555	41.60	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.20%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	24966	4.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.20%
64) 1,2-Dichlorobenzene-d4	11.65	152	40415	4.99	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.80%

Target Compounds


					Ovalue
13) Acetone	2.20	43	9116	8.283 ug/L	# 56
25) Chloroform	4.41	83	13019	0.892 ug/L	97
47) Tetrachloroethene	8.00	164	452840	74.318 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV041420\
Data File : VV015494.D
Acq On : 15 Apr 2020 04:31
Operator : SY/MD
Sample : L2274-14
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAQB2

Quant Time: Apr 15 07:07:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 15 05:31:01 2020
Response via : Initial Calibration

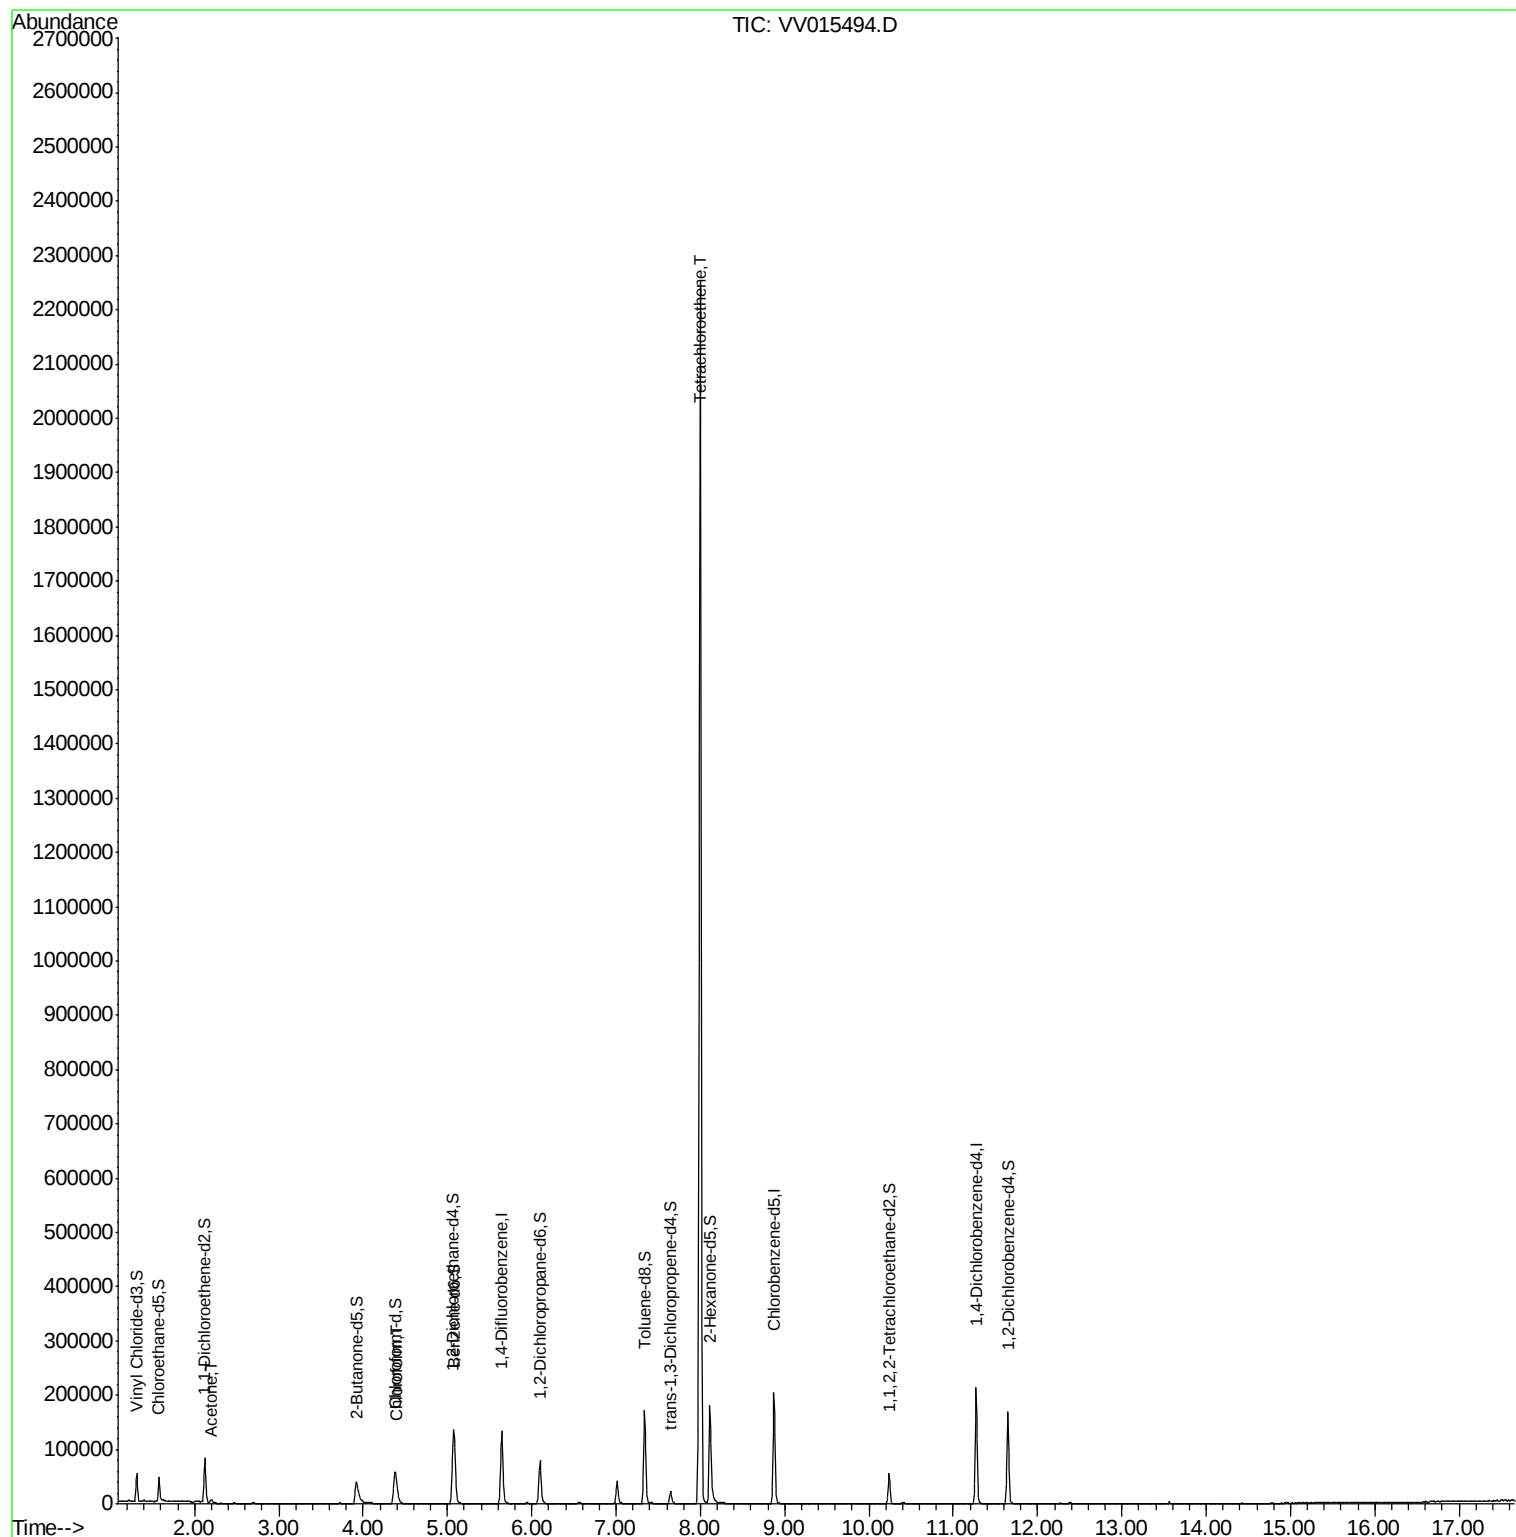

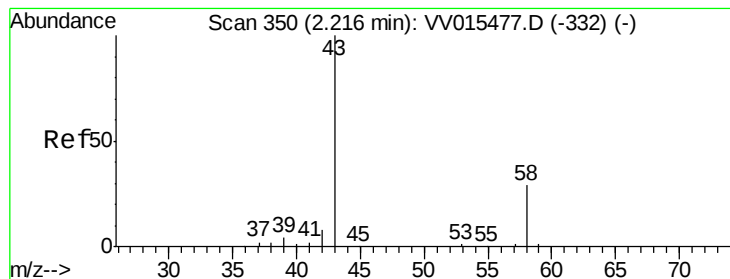

#13

Acetone

Concen: 8.283 ug/L

RT: 2.20 min Scan# 344

Delta R.T. -0.02 min

Lab File: VV015494.D

Acq: 15 Apr 2020 04:31

Instrument :

MSVOA_V

ClientSampleId :


YaqB2

Tot Ion: 43 Resp: 9116

Ion Ratio Lower Upper




43 100

58 27.7 0.0 22.2#

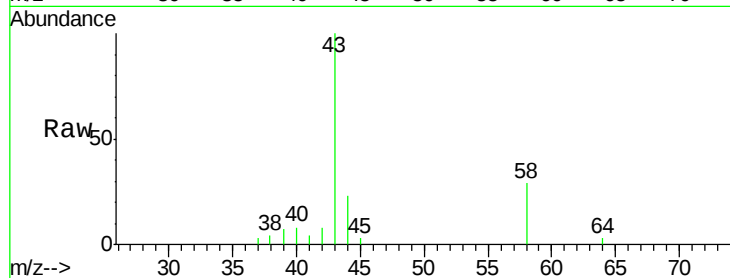

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

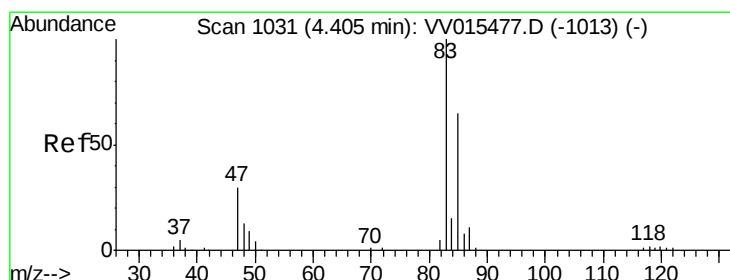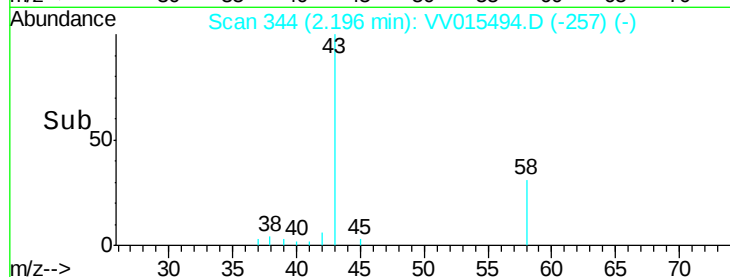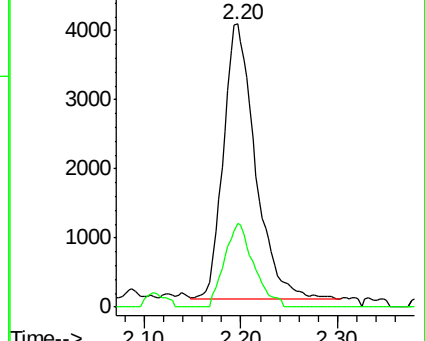

#25

Chloroform

Concen: 0.892 ug/L

RT: 4.41 min Scan# 1032

Delta R.T. 0.00 min

Lab File: VV015494.D


Acq: 15 Apr 2020 04:31

Tgt Ion: 83 Resp: 13019

Ion Ratio Lower Upper



83 100


85 63.0 45.9 85.3

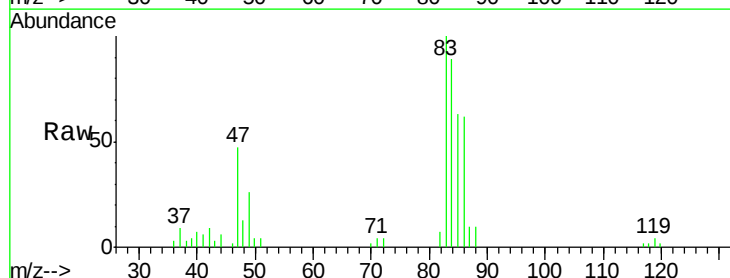

Abundance Ion 83.05 (82.75 to 83.75): VV0

Ion 85.00 (84.70 to 85.70): VV0

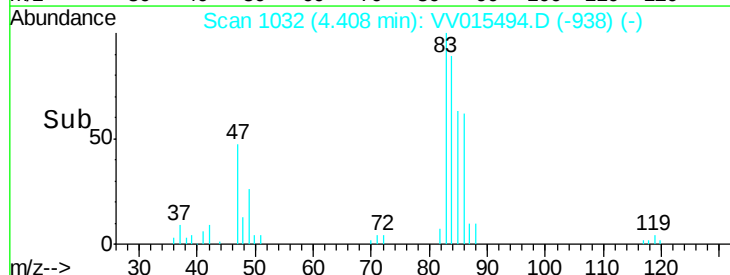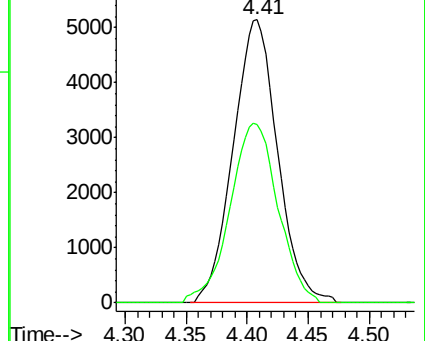

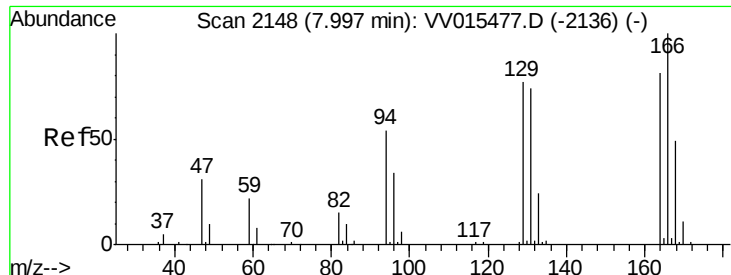

#47

Tetrachloroethene

Concen: 74.318 ug/L

RT: 8.00 min Scan# 2148

Delta R.T. 0.00 min

Lab File: VV015494.D


Acq: 15 Apr 2020 04:31

Instrument :

MSVOA_V

ClientSampleId :

YaqB2

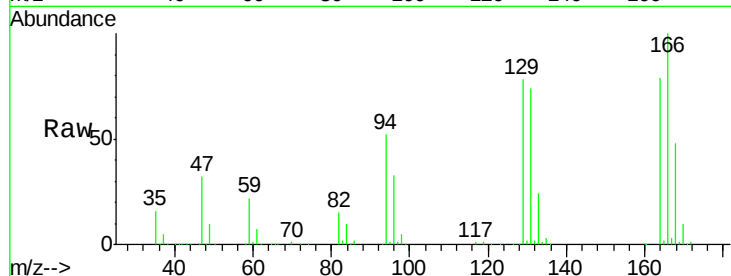

Tot Ion:164 Resp: 452840

Ion Ratio Lower Upper

164 100

129 98.9 70.6 131.0

131 94.1 68.3 126.8

166 126.9 88.3 163.9

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

