

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041420\
 Data File : VV015497.D
 Acq On : 15 Apr 2020 05:41
 Operator : SY/MD
 Sample : L2274-17
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YaqB5

Quant Time: Apr 15 07:25:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 15 05:31:01 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	107757	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	101283	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	50284	5.00	ug/L	0.00


System Monitoring Compounds


4) Vinyl Chloride-d3	1.31	65	30880	5.52	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	110.40%
7) Chloroethane-d5	1.58	69	26949	5.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.80%
11) 1,1-Dichloroethene-d2	2.12	63	44535	3.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.60%
20) 2-Butanone-d5	3.92	46	74702	47.58		

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV041420\
Data File : VV015497.D
Acq On : 15 Apr 2020 05:41
Operator : SY/MD
Sample : L2274-17
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YaqB5

Quant Time: Apr 15 07:25:43 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 15 05:31:01 2020
Response via : Initial Calibration

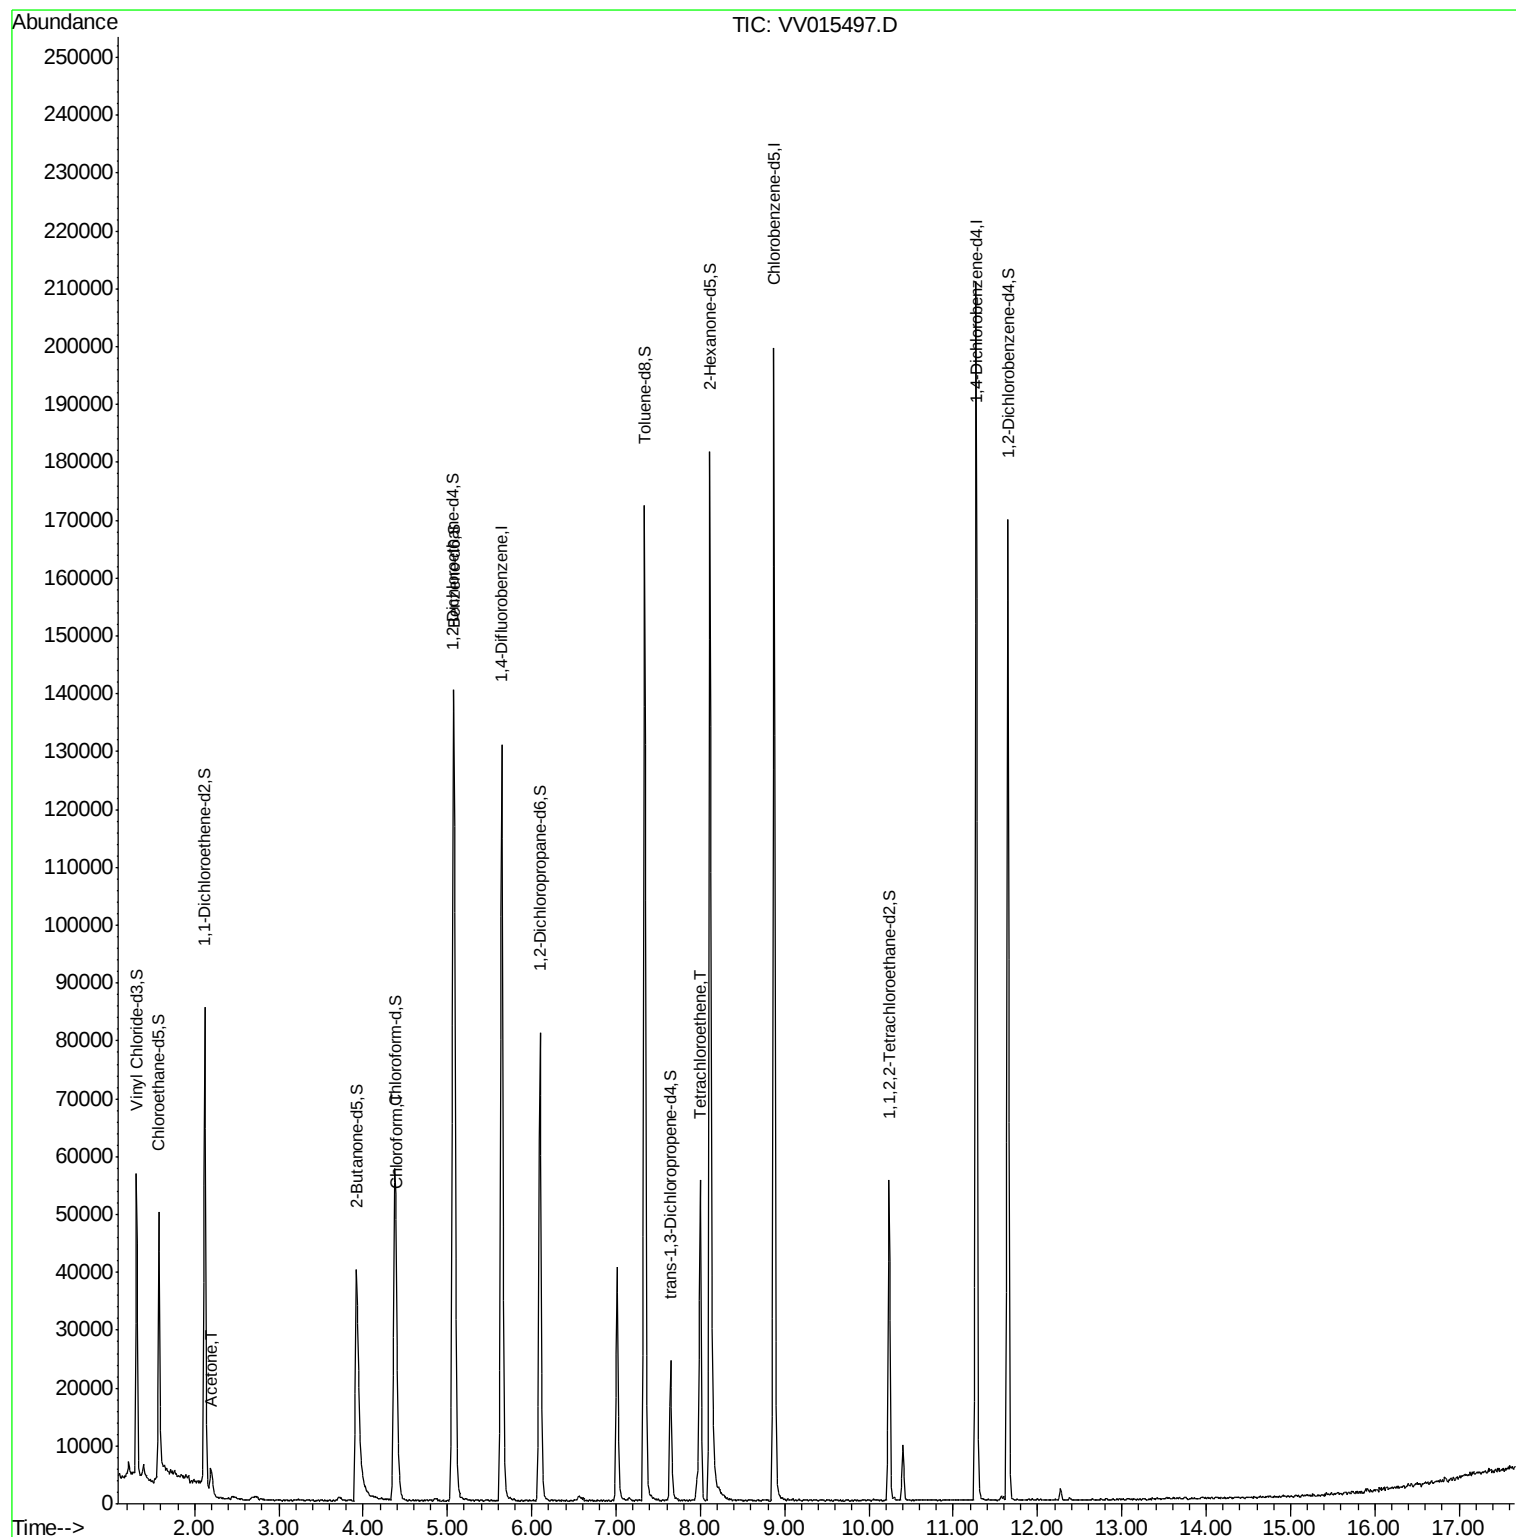

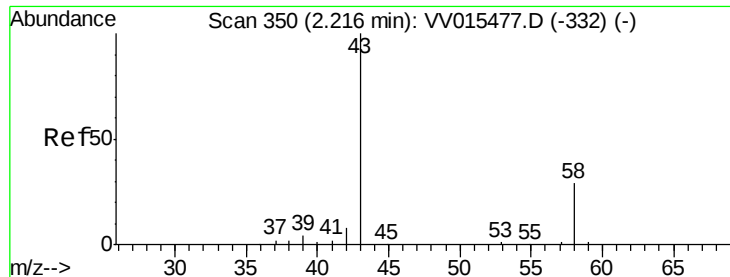

#13

Acetone

Concen: 6.192 ug/L

RT: 2.20 min Scan# 344

Delta R.T. -0.02 min

Lab File: VV015497.D

Acq: 15 Apr 2020 05:41

Instrument :

MSVOA_V

ClientSampled :


YaqB5

Tot Ion: 43 Resp: 6868

Ion Ratio Lower Upper




43 100


58 30.7 0.0 22.2#

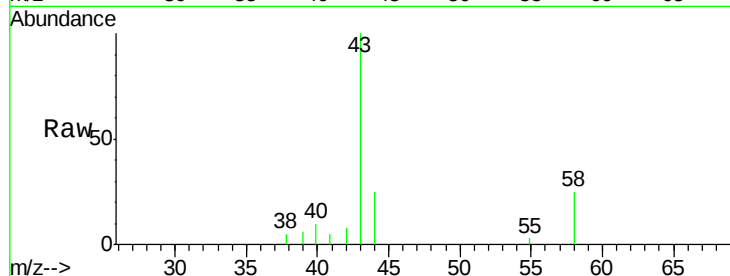

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

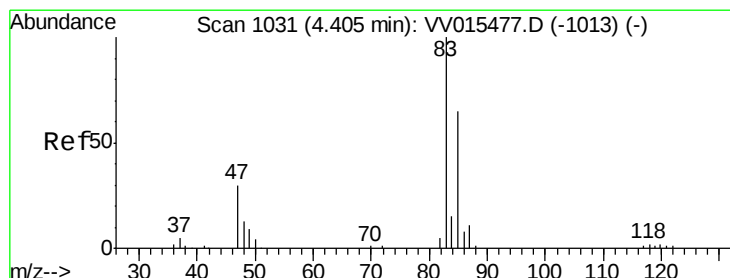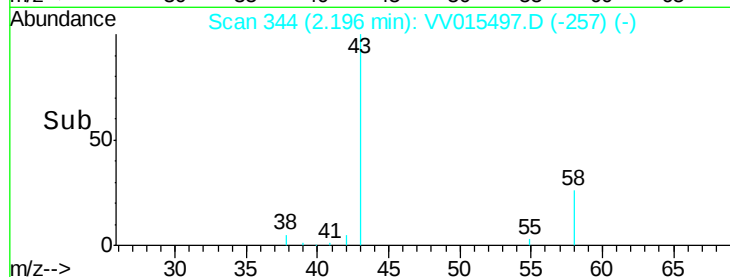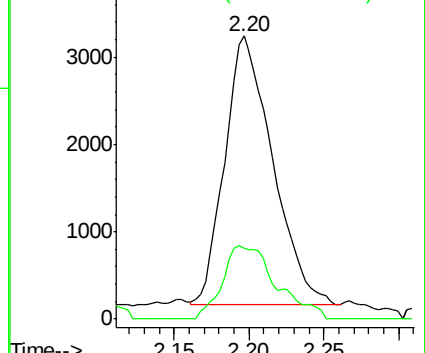

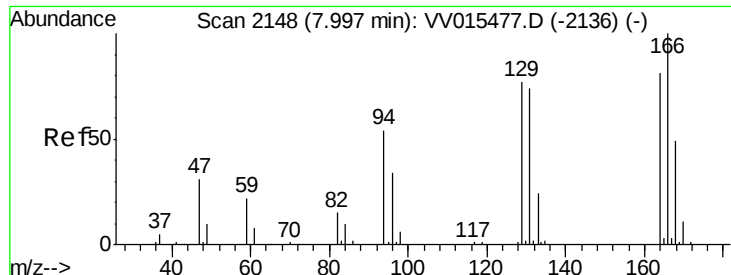

#47

Tetrachloroethene

Concen: 1.939 ug/L

RT: 8.00 min Scan# 2148

Delta R.T. 0.00 min

Lab File: VV015497.D


Acq: 15 Apr 2020 05:41

Instrument :

MSVOA_V

ClientSampleId :

YaqB5

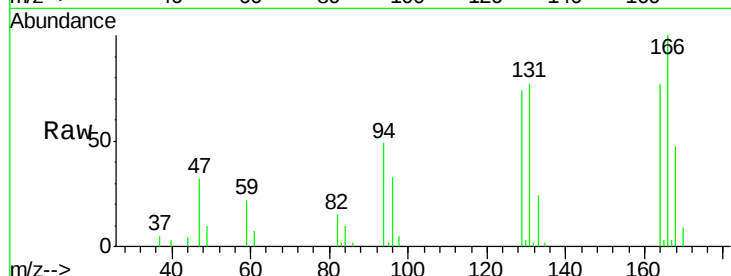

Tot Ion:164 Resp: 11724

Ion Ratio Lower Upper

164 100

129 95.4 70.6 131.0

131 99.5 68.3 126.8

166 129.6 88.3 163.9

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V