


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV041420\
Data File : VV015456.D
Acq On : 14 Apr 2020 10:06
Operator : SY/MD
Sample : BFB34
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB34

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Apr 15 05:31:01 2020

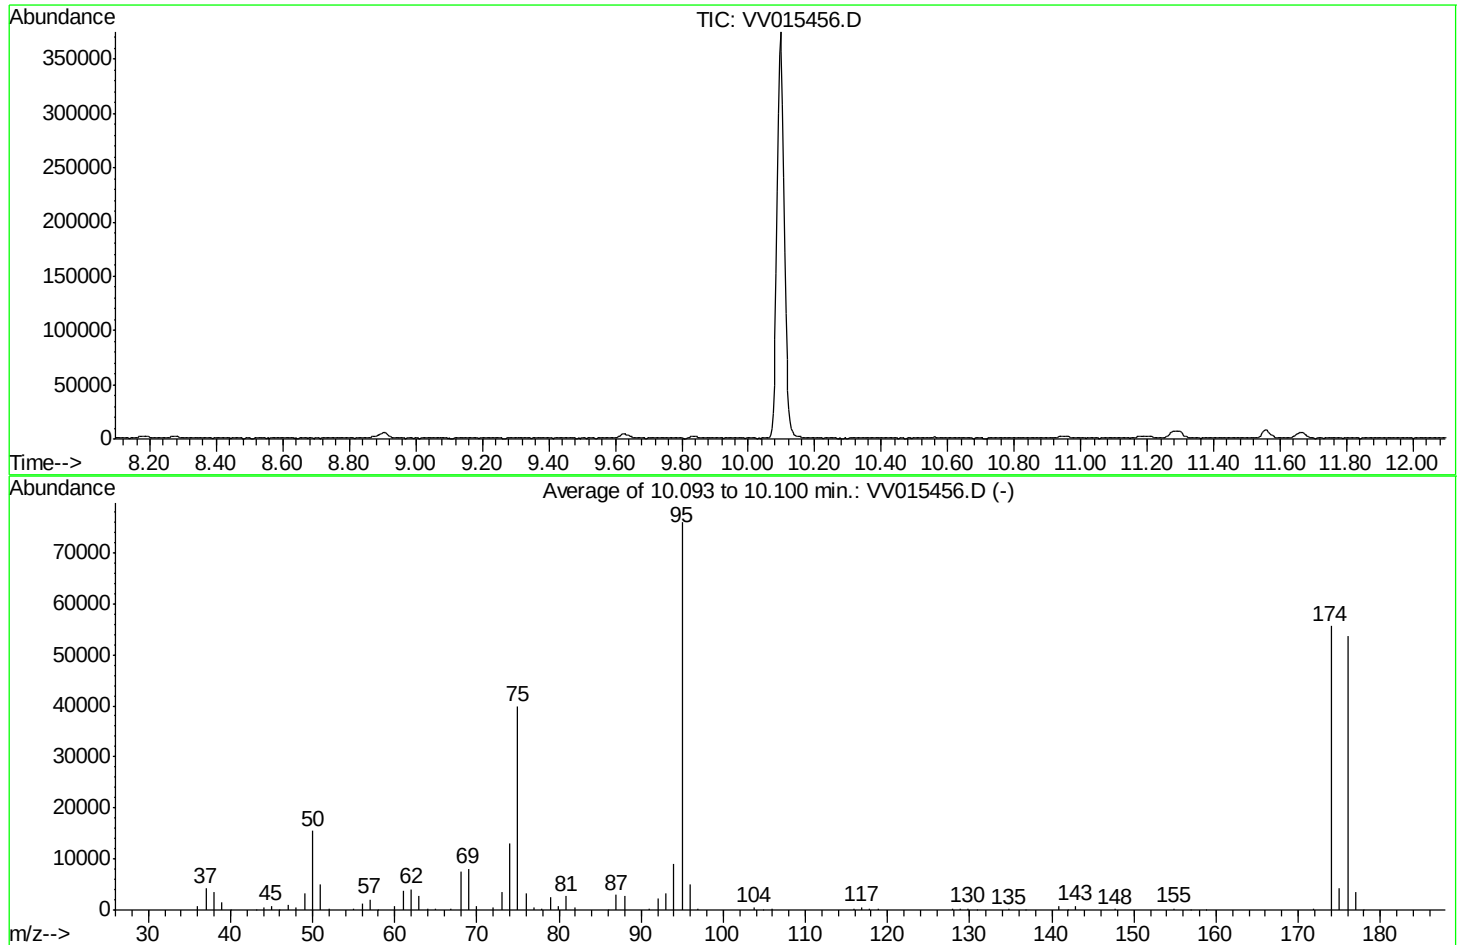

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	15446	PASS
75	95	30	80	52.5	39834	PASS
95	95	100	100	100.0	75941	PASS
96	95	5	9	6.8	5139	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.2	55594	PASS
175	174	5	9	7.7	4265	PASS
176	174	95	101	96.3	53549	PASS
177	176	5	9	6.4	3442	PASS

m/z	Abundance
36.00	780.0
37.00	4222.0
38.00	3639.0
39.00	1356.0
40.00	308.0
43.20	129.0
44.00	730.0
44.90	783.0
47.00	947.0
48.00	517.0
49.00	3400.0
50.00	15583.0
51.00	4981.0
52.00	218.0
55.00	282.0
56.00	1234.0
57.00	2005.0
57.90	121.0
60.00	796.0
61.00	3729.0
62.00	3927.0
63.00	2746.0
64.00	264.0
64.90	200.0
66.90	189.0
68.00	7427.0
69.00	8080.0
70.00	613.0
72.00	482.0
73.00	3557.0
74.00	12888.0
75.00	39296.0
76.00	3344.0
76.90	485.0
78.00	315.0
78.90	2429.0
79.90	777.0
80.90	2660.0
81.90	586.0
86.10	125.0
87.00	2873.0
88.00	2705.0
90.90	273.0
92.00	2256.0
93.00	3128.0
94.00	8750.0
95.00	74808.0
96.00	5203.0
97.00	184.0
103.80	364.0
104.90	124.0
105.90	349.0
115.90	365.0
116.90	484.0
117.90	301.0
118.90	361.0
127.90	264.0
128.90	144.0
129.80	304.0
134.80	144.0
136.80	119.0
140.90	684.0
141.90	101.0
142.90	865.0
147.80	150.0
154.90	309.0
156.90	104.0
158.80	110.0
171.80	269.0
174.00	52728.0
175.00	4183.0
176.00	50936.0
177.00	3472.0
177.90	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

m/z	Abundance
36.00	914.0
37.00	4306.0
38.00	3709.0
39.00	1455.0
40.00	330.0
43.20	131.0
44.00	770.0
45.00	817.0
45.90	117.0
47.00	947.0
48.00	526.0
49.00	3471.0
50.00	15933.0
51.00	5258.0
52.00	236.0
55.00	297.0
56.00	1322.0
57.00	2073.0
57.90	142.0
60.00	860.0
61.00	3801.0
62.00	4252.0
63.00	2862.0
64.00	277.0
64.90	192.0
66.90	219.0
68.00	7862.0
69.00	8463.0
70.00	656.0
72.00	507.0
73.00	3740.0
74.00	13598.0
75.00	41184.0
76.00	3485.0
77.00	424.0
77.90	368.0
78.90	2570.0
79.90	792.0
80.90	2753.0
81.90	633.0
85.90	111.0
86.10	113.0
86.90	3033.0
88.00	2809.0
90.90	297.0
92.00	2367.0
93.00	3331.0
94.00	9343.0
95.00	78576.0
96.00	5343.0
97.00	199.0
103.80	423.0
104.90	105.0
105.90	370.0
115.90	372.0
116.80	529.0
117.80	332.0
118.90	376.0
127.90	269.0
128.80	152.0
129.80	305.0
130.80	113.0
134.80	154.0
136.80	116.0
140.90	770.0
141.80	115.0
142.90	890.0
147.70	181.0
154.90	273.0
156.90	140.0
158.80	103.0
171.90	283.0
174.00	57512.0
175.00	4392.0
176.00	55496.0
177.00	3562.0
177.90	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

m/z	Abundance
36.00	882.0
37.00	3965.0
38.00	3396.0
39.00	1356.0
40.00	333.0
43.10	124.0
44.00	748.0
45.00	749.0
45.90	118.0
47.00	892.0
48.00	481.0
49.00	3267.0
50.00	14824.0
51.00	4901.0
52.00	230.0
55.00	296.0
56.00	1230.0
57.00	1988.0
57.90	132.0
60.00	811.0
61.00	3582.0
62.00	3985.0
63.00	2693.0
64.00	292.0
64.90	158.0
66.80	243.0
68.00	7477.0
69.00	7914.0
70.00	653.0
71.90	499.0
73.00	3417.0
74.00	12754.0
75.00	39024.0
76.00	3299.0
77.00	373.0
77.90	361.0
78.90	2380.0
79.90	722.0
80.90	2537.0
81.90	578.0
87.00	2862.0
88.00	2671.0
90.90	299.0
92.00	2228.0
93.00	3195.0
94.00	8971.0
95.00	74440.0
96.00	4873.0
96.90	196.0
103.80	414.0
105.90	358.0
115.90	330.0
116.90	510.0
117.80	313.0
118.80	345.0
127.80	269.0
128.80	159.0
129.80	271.0
130.80	132.0
134.80	147.0
136.70	108.0
140.90	823.0
141.80	110.0
142.90	826.0
147.80	181.0
154.90	201.0
156.90	141.0
172.00	261.0
174.00	56544.0
175.00	4221.0
176.00	54216.0
177.00	3293.0
177.90	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

Scan 2788 (10.055 min): VV015456.D
BFB34

m/z	Abundance
39.90	281.0
41.10	122.0
42.90	119.0
44.00	312.0
54.90	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34