

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021012.D
 Acq On : 14 Apr 2021 17:47
 Operator : SY/MD
 Sample : M2031-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 15 03:06:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 15 01:36:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	440614	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	423457	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	202072	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	116636	48.66	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 97.32%			
7) Chloroethane-d5	1.571	69	96562	51.24	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 102.48%			
11) 1,1-Dichloroethene-d2	2.108	63	189819	36.92	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 73.84%			
21) 2-Butanone-d5	3.896	46	184809	117.24	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 117.24%			
24) Chloroform-d	4.352	84	299841	50.39	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.78%			
26) 1,2-Dichloroethane-d4	5.034	65	211922	52.69	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 105.38%			
32) Benzene-d6	5.053	84	556992	53.28	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 106.56%			
36) 1,2-Dichloropropane-d6	6.075	67	156981	54.08	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 108.16%			
41) Toluene-d8	7.320	98	534098	51.55	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 103.10%			
43) trans-1,3-Dichloroprop...	7.625	79	89842	50.23	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 100.46%			
47) 2-Hexanone-d5	8.091	63	161992	129.93	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 129.93%			
56) 1,1,2,2-Tetrachloroeth...	10.220	84	249411	53.02	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 106.04%			
66) 1,2-Dichlorobenzene-d4	11.632	152	228203	55.32	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 110.64%			
Target Compounds					Qvalue	
25) Chloroform	4.384	83	12854	2.10	ug/L	92
42) Toluene	7.400	91	17200	1.44	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021012.D
Acq On : 14 Apr 2021 17:47
Operator : SY/MD
Sample : M2031-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Apr 15 03:06:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 15 01:36:39 2021
Response via : Initial Calibration

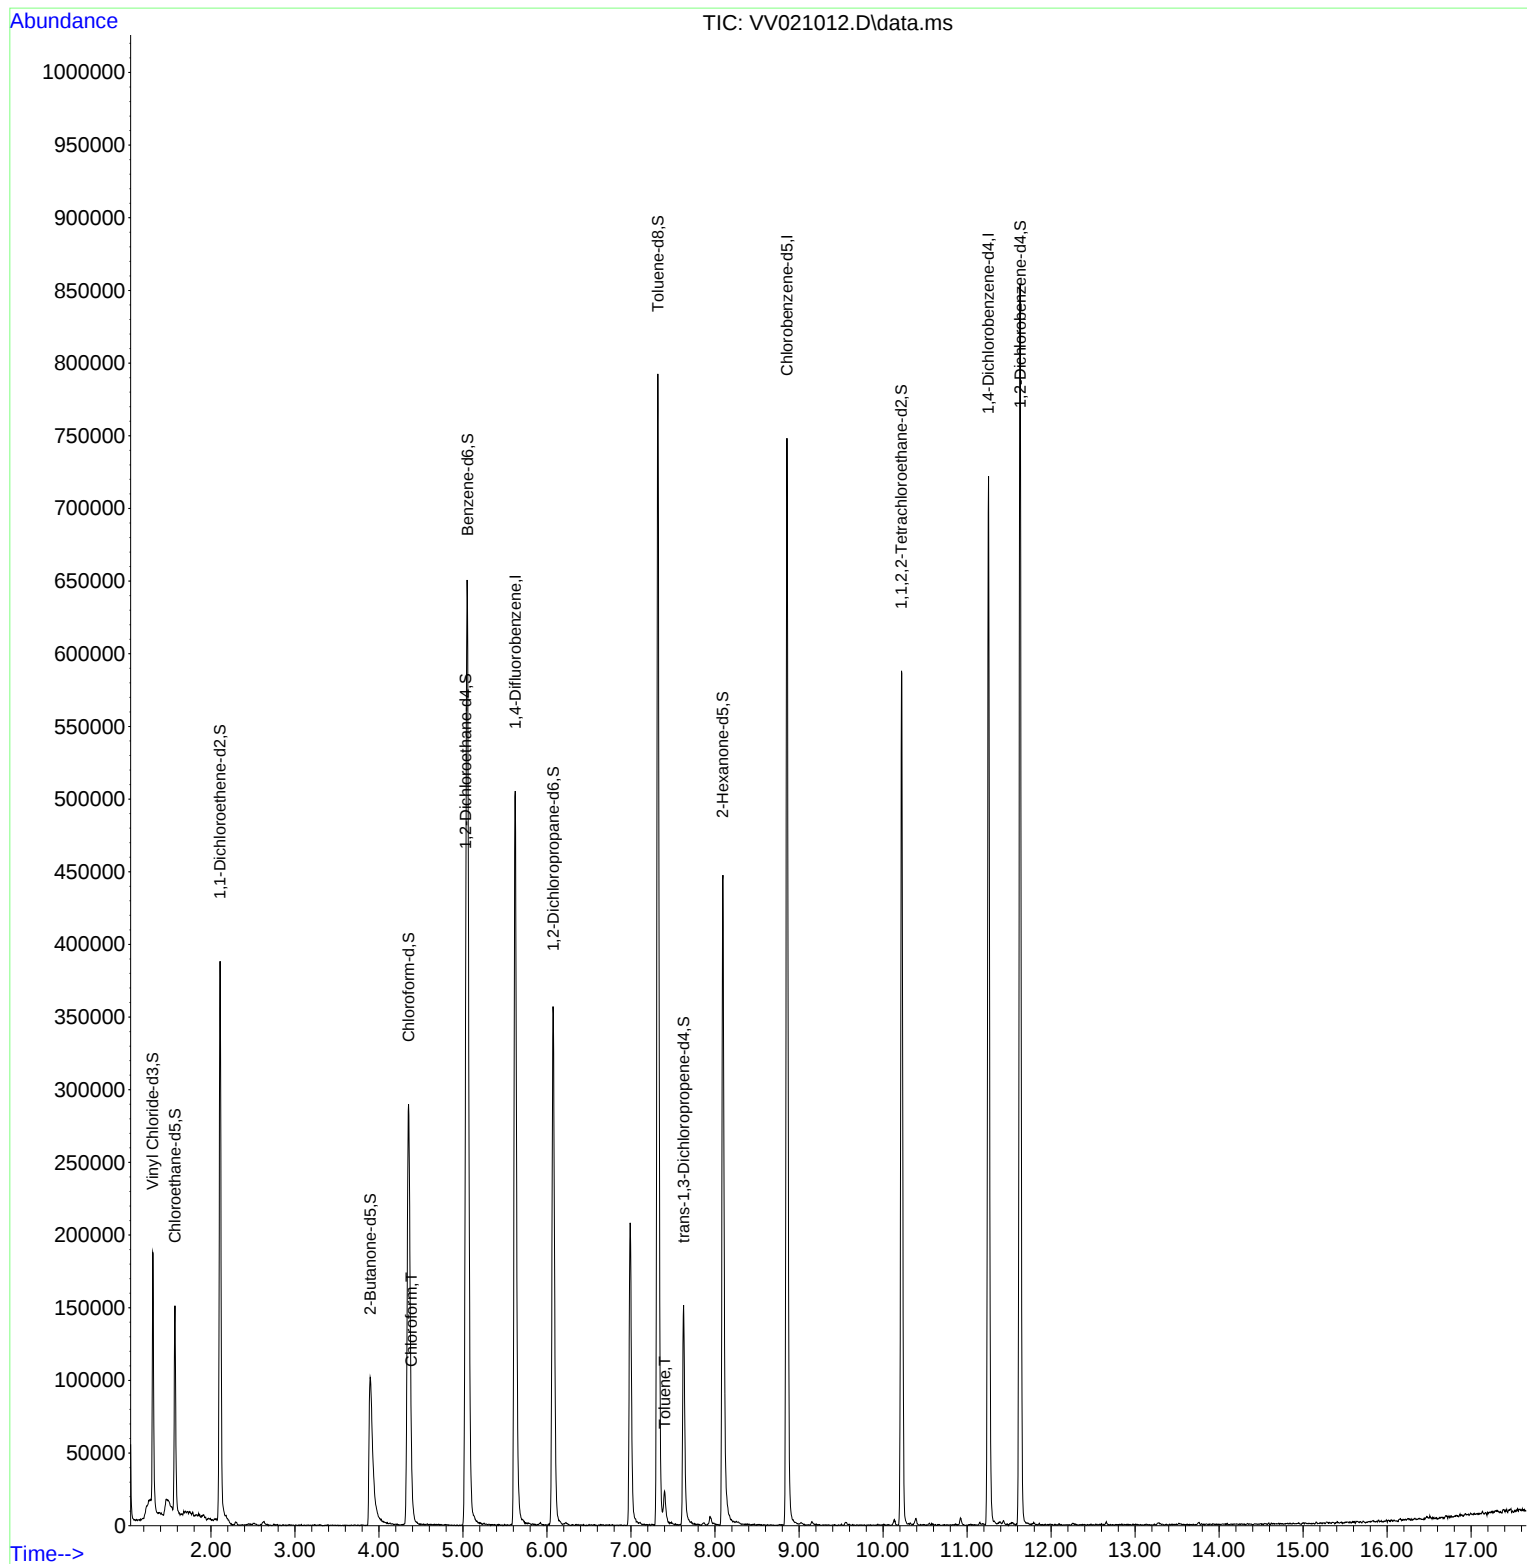




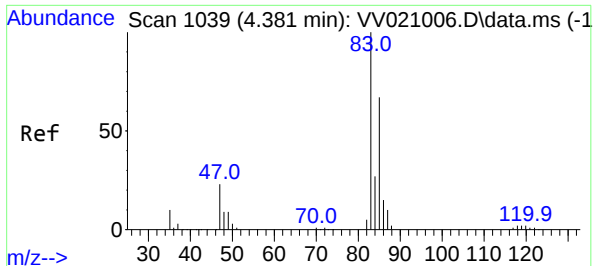


#25

Chloroform
Concen: 2.10 ug/L
RT: 4.384 min Scan# 1040
Delta R.T. 0.003 min
Lab File: VV021012.D
Acq: 14 Apr 2021 17:47

Instrument :
MSVOA_V
ClientSampled :

Tgt Ion: 83 Resp: 12854
Ion Ratio Lower Upper
83 100
85 73.2 46.6 86.6

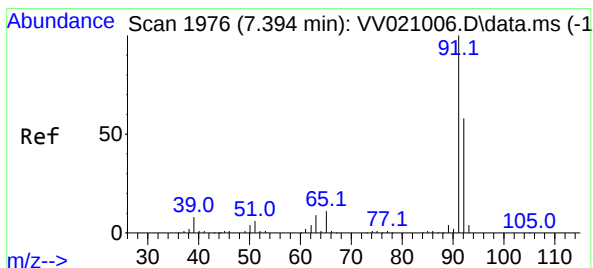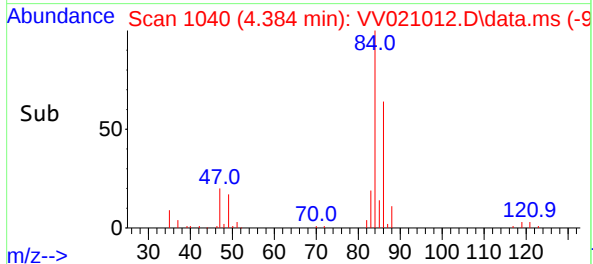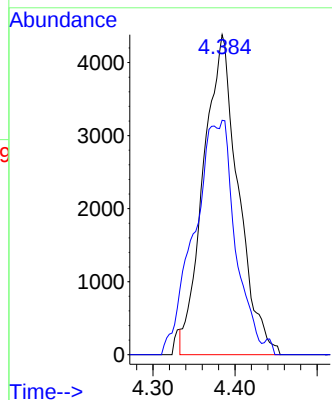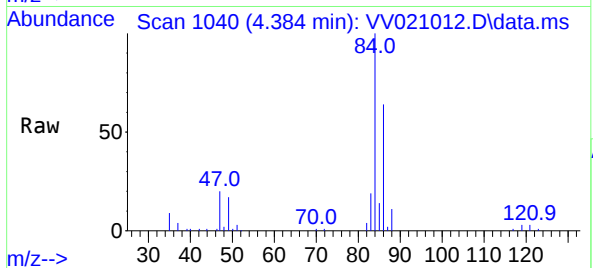

#42

Toluene
Concen: 1.44 ug/L
RT: 7.400 min Scan# 1978
Delta R.T. 0.006 min
Lab File: VV021012.D
Acq: 14 Apr 2021 17:47

Tgt Ion: 91 Resp: 17200
Ion Ratio Lower Upper
91 100
92 55.2 40.5 75.3

