

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021010.D
 Acq On : 14 Apr 2021 17:00
 Operator : SY/MD
 Sample : VV0414WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK163

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M

Title : VOC Analysis

Signal : TIC: VV021010.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	78	84	101	rVB	198961	218368	12.37%	1.589%
2	1.571	159	165	182	rVB	158052	201454	11.41%	1.466%
3	2.111	323	333	362	rVB	411790	612606	34.69%	4.458%
4	2.298	384	391	398	rVB2	3727	4888	0.28%	0.036%
5	2.372	410	414	415	rBV3	672	382	0.02%	0.003%
6	2.513	449	458	467	rBV6	2463	4404	0.25%	0.032%
7	2.658	502	503	506	rBV	338	194	0.01%	0.001%
8	2.690	512	513	519	rVB	429	241	0.01%	0.002%
9	2.767	531	537	544	rVB7	1378	1845	0.10%	0.013%
10	2.815	550	552	555	rBV	401	238	0.01%	0.002%
11	2.970	597	600	601	rBV	405	240	0.01%	0.002%
12	2.995	605	608	610	rBV2	288	238	0.01%	0.002%
13	3.092	634	638	640	rBV	288	225	0.01%	0.002%
14	3.333	710	713	718	rBV2	524	398	0.02%	0.003%
15	3.545	777	779	781	rVV	652	275	0.02%	0.002%
16	3.590	791	793	795	rVB2	369	192	0.01%	0.001%
17	3.609	795	799	803	rBV	392	346	0.02%	0.003%
18	3.735	835	838	840	rBV	309	262	0.01%	0.002%
19	3.860	874	877	880	rBV3	509	284	0.02%	0.002%
20	3.902	880	890	932	rBV2	87927	309087	17.50%	2.249%
21	4.352	1014	1030	1061	rBV	304006	775346	43.91%	5.643%
22	4.616	1109	1112	1113	rBV	700	297	0.02%	0.002%
23	4.664	1125	1127	1131	rBV3	646	346	0.02%	0.003%
24	4.925	1204	1208	1209	rBV2	412	297	0.02%	0.002%
25	4.979	1223	1225	1227	rBV2	592	277	0.02%	0.002%
26	5.050	1230	1247	1280	rVV2	685748	1765905	100.00%	12.851%
27	5.326	1331	1333	1336	rBV2	792	411	0.02%	0.003%
28	5.365	1340	1345	1346	rBV2	994	572	0.03%	0.004%
29	5.429	1362	1365	1367	rBV3	423	233	0.01%	0.002%
30	5.461	1373	1375	1379	rVB	460	339	0.02%	0.002%
31	5.500	1383	1387	1388	rBV	447	298	0.02%	0.002%
32	5.542	1394	1400	1402	rBV3	655	777	0.04%	0.006%
33	5.622	1409	1425	1452	rBV	547520	1113804	63.07%	8.106%
34	5.908	1511	1514	1516	rBV4	1924	1352	0.08%	0.010%
35	5.986	1534	1538	1539	rBV2	669	345	0.02%	0.003%
36	6.076	1550	1566	1587	rBV	378088	762594	43.18%	5.550%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021010.D
 Acq On : 14 Apr 2021 17:00
 Operator : SY/MD
 Sample : VV0414WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK163

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.297	1633	1635	1637	rBV2	684	260	0.01%	0.002%
38	6.307	1637	1638	1642	rVV	542	203	0.01%	0.001%
39	6.339	1646	1648	1651	rVB	391	195	0.01%	0.001%
40	6.394	1659	1665	1668	rBV3	586	593	0.03%	0.004%
41	6.413	1668	1671	1674	rVB2	318	211	0.01%	0.002%
42	6.478	1689	1691	1695	rBV	589	336	0.02%	0.002%
43	6.503	1695	1699	1703	rVB	435	438	0.02%	0.003%
44	6.619	1732	1735	1737	rVV2	627	284	0.02%	0.002%
45	6.648	1740	1744	1748	rBV3	784	687	0.04%	0.005%
46	6.760	1776	1779	1783	rBV2	363	349	0.02%	0.003%
47	6.786	1785	1787	1791	rVB2	491	323	0.02%	0.002%
48	6.812	1792	1795	1799	rBV	511	518	0.03%	0.004%
49	6.834	1799	1802	1803	rBV2	374	195	0.01%	0.001%
50	6.863	1808	1811	1814	rVB2	275	203	0.01%	0.001%
51	6.989	1839	1850	1871	rBV	230563	412483	23.36%	3.002%
52	7.214	1917	1920	1925	rVB3	625	418	0.02%	0.003%
53	7.252	1928	1932	1936	rBV4	693	632	0.04%	0.005%
54	7.320	1940	1953	1971	rBV	857347	1483977	84.03%	10.800%
55	7.625	2038	2048	2065	rBV2	163037	282043	15.97%	2.053%
56	7.944	2141	2147	2150	rBV3	1364	1618	0.09%	0.012%
57	8.095	2183	2194	2216	rBV	406387	721853	40.88%	5.253%
58	8.654	2360	2368	2370	rBV2	496	529	0.03%	0.004%
59	8.715	2383	2387	2388	rBV2	693	443	0.03%	0.003%
60	8.783	2405	2408	2409	rBV	463	252	0.01%	0.002%
61	8.857	2420	2431	2454	rBV	826982	1342122	76.00%	9.767%
62	9.108	2506	2509	2514	rVB2	538	328	0.02%	0.002%
63	9.214	2539	2542	2544	rBV	534	292	0.02%	0.002%
64	9.230	2545	2547	2550	rVV	441	246	0.01%	0.002%
65	9.336	2577	2580	2587	rBV3	431	460	0.03%	0.003%
66	9.365	2587	2589	2595	rVB3	636	543	0.03%	0.004%
67	9.397	2595	2599	2602	rBV3	634	441	0.02%	0.003%
68	9.413	2602	2604	2606	rBV	527	311	0.02%	0.002%
69	9.510	2632	2634	2636	rBV	461	243	0.01%	0.002%
70	9.645	2673	2676	2678	rBV	425	243	0.01%	0.002%
71	9.680	2684	2687	2691	rBV3	457	268	0.02%	0.002%
72	9.699	2691	2693	2695	rBV	348	210	0.01%	0.002%
73	9.911	2755	2759	2763	rVB2	597	515	0.03%	0.004%
74	9.944	2763	2769	2773	rBV3	1228	1632	0.09%	0.012%
75	10.082	2809	2812	2815	rBV2	342	215	0.01%	0.002%
76	10.137	2819	2829	2837	rVB4	4286	6197	0.35%	0.045%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021010.D
 Acq On : 14 Apr 2021 17:00
 Operator : SY/MD
 Sample : VV0414WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK163

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.172	2837	2840	2842	rBV2	772	382	0.02%	0.003%
78	10.220	2843	2855	2873	rBV	594094	932333	52.80%	6.785%
79	10.464	2929	2931	2934	rVB2	833	323	0.02%	0.002%
80	10.548	2955	2957	2961	rBV3	1025	763	0.04%	0.006%
81	10.702	3003	3005	3007	rBV2	407	207	0.01%	0.002%
82	10.924	3067	3074	3082	rVV6	3735	5905	0.33%	0.043%
83	10.960	3082	3085	3093	rVB3	711	862	0.05%	0.006%
84	11.153	3141	3145	3151	rVB4	1548	1569	0.09%	0.011%
85	11.255	3166	3177	3199	rBV	831212	1289030	73.00%	9.381%
86	11.464	3239	3242	3244	rBV3	527	314	0.02%	0.002%
87	11.577	3271	3277	3281	rBV4	1216	1449	0.08%	0.011%
88	11.632	3282	3294	3317	rVV	943470	1457895	82.56%	10.610%
89	11.857	3361	3364	3372	rVB4	1216	1306	0.07%	0.010%
90	11.921	3383	3384	3388	rBV2	354	199	0.01%	0.001%
91	11.989	3400	3405	3409	rBV2	683	579	0.03%	0.004%
92	12.046	3421	3423	3425	rBV	410	215	0.01%	0.002%
93	12.246	3483	3485	3487	rBV	508	206	0.01%	0.001%
94	12.744	3638	3640	3643	rBV2	435	199	0.01%	0.001%
95	12.821	3661	3664	3668	rBV2	646	598	0.03%	0.004%
96	13.017	3722	3725	3727	rBV2	540	343	0.02%	0.002%
97	13.432	3852	3854	3855	rBV	532	252	0.01%	0.002%
98	13.606	3905	3908	3912	rBV2	881	753	0.04%	0.005%
99	13.751	3949	3953	3954	rBV3	3130	2095	0.12%	0.015%
100	14.136	4070	4073	4077	rBV3	758	699	0.04%	0.005%




Sum of corrected areas: 13741145

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021010.D
Acq On : 14 Apr 2021 17:00
Operator : SY/MD
Sample : VV0414WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK163

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

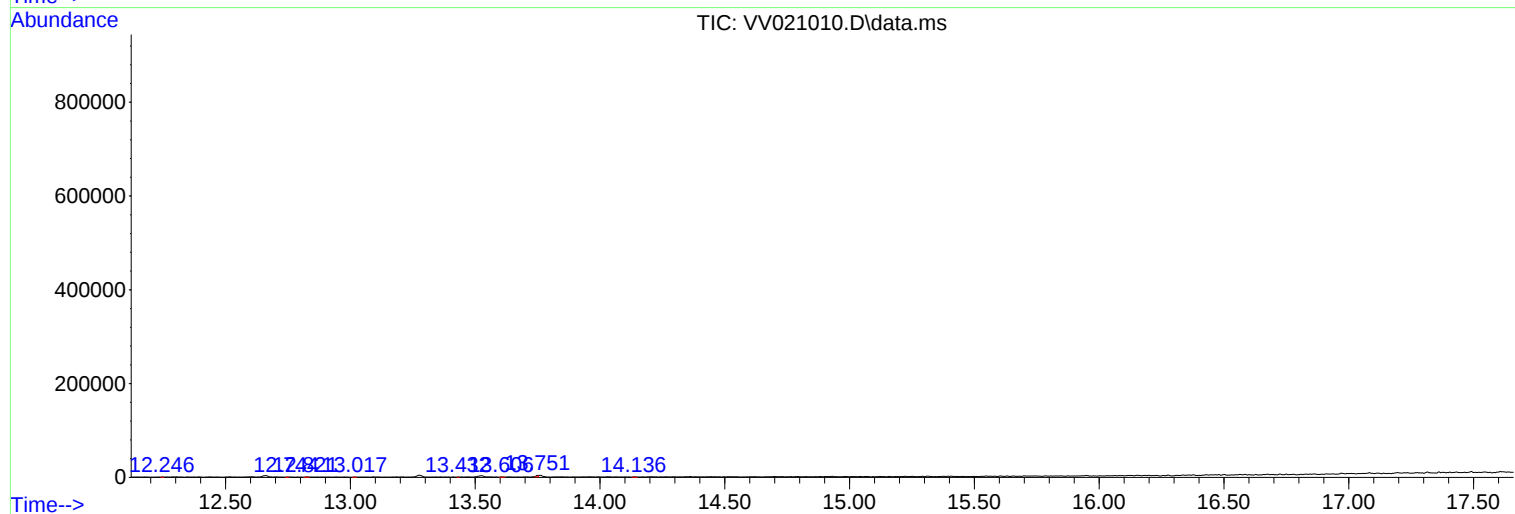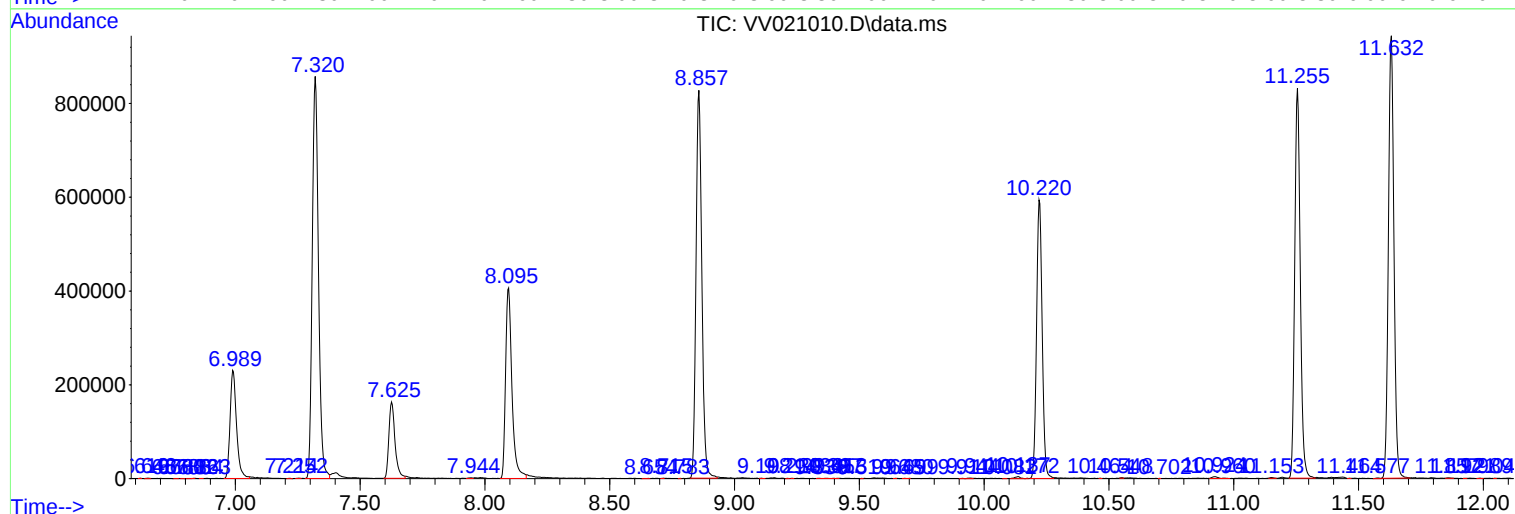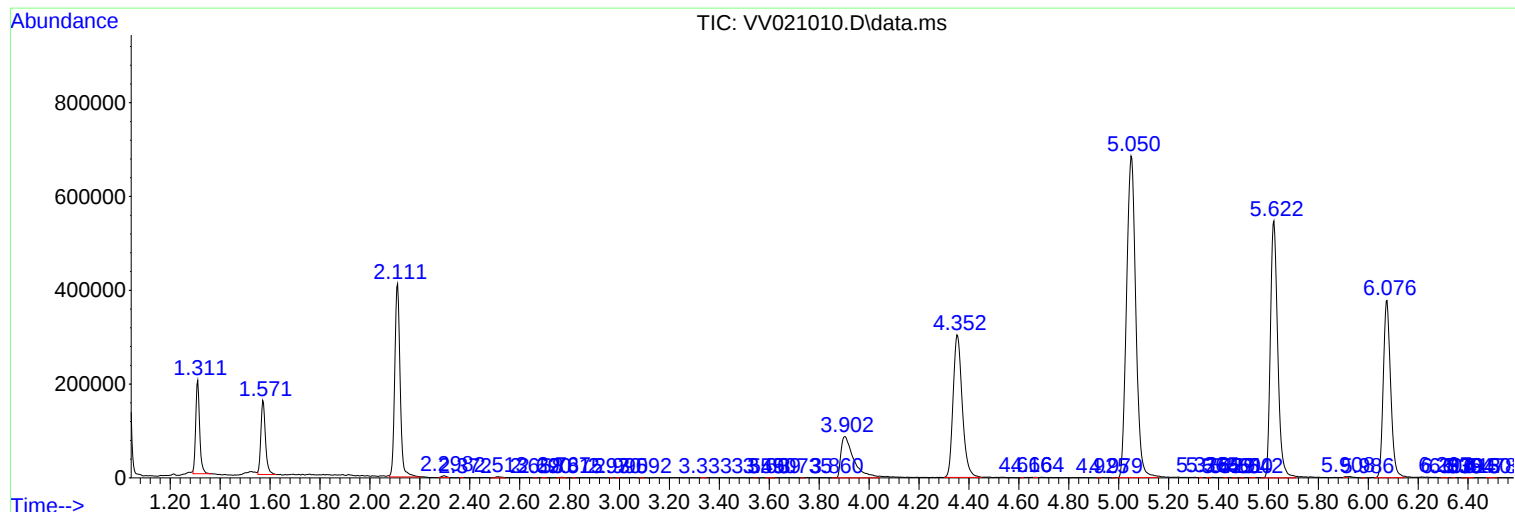

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021010.D
Acq On : 14 Apr 2021 17:00
Operator : SY/MD
Sample : VV0414WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK163

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021010.D
Acq On : 14 Apr 2021 17:00
Operator : SY/MD
Sample : VV0414WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK163

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
