

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021012.D
 Acq On : 14 Apr 2021 17:47
 Operator : SY/MD
 Sample : M2031-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG528

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

Signal : TIC: VV021012.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	78	83	104	rVB	179779	206356	12.30%	1.599%
2	1.571	159	165	180	rVB	143091	177866	10.60%	1.378%
3	2.108	323	332	351	rBV	382470	550417	32.81%	4.266%
4	2.294	386	390	397	rVB2	1982	2684	0.16%	0.021%
5	2.474	444	446	450	rBV2	720	328	0.02%	0.003%
6	2.503	452	455	458	rBV4	890	814	0.05%	0.006%
7	2.632	485	495	500	rVV2	2353	3984	0.24%	0.031%
8	2.748	524	531	536	rBV3	1091	1436	0.09%	0.011%
9	2.847	559	562	563	rBV	424	263	0.02%	0.002%
10	2.915	580	583	585	rBV	397	282	0.02%	0.002%
11	2.928	585	587	590	rVV2	514	353	0.02%	0.003%
12	2.963	594	598	600	rBV2	342	297	0.02%	0.002%
13	3.011	608	613	616	rBV	447	370	0.02%	0.003%
14	3.076	631	633	638	rVB3	758	354	0.02%	0.003%
15	3.108	641	643	648	rVB2	382	265	0.02%	0.002%
16	3.233	680	682	685	rVB2	513	289	0.02%	0.002%
17	3.269	689	693	697	rBV	290	266	0.02%	0.002%
18	3.355	717	720	722	rBV	405	289	0.02%	0.002%
19	3.667	813	817	820	rBV2	547	487	0.03%	0.004%
20	3.709	825	830	835	rBV2	398	551	0.03%	0.004%
21	3.789	849	855	857	rBV2	519	623	0.04%	0.005%
22	3.896	877	888	926	rBV	101810	329698	19.65%	2.555%
23	4.352	1015	1030	1059	rBV	288624	728299	43.41%	5.644%
24	4.629	1114	1116	1118	rBV3	536	262	0.02%	0.002%
25	4.741	1147	1151	1154	rBV4	566	450	0.03%	0.003%
26	4.870	1187	1191	1195	rVB	348	302	0.02%	0.002%
27	4.928	1205	1209	1214	rBB3	560	517	0.03%	0.004%
28	4.960	1215	1219	1222	rBV2	497	405	0.02%	0.003%
29	4.982	1222	1226	1230	rBV3	341	295	0.02%	0.002%
30	5.050	1230	1247	1281	rBV2	650488	1677563	100.00%	13.001%
31	5.346	1337	1339	1344	rVV2	489	379	0.02%	0.003%
32	5.490	1380	1384	1387	rBV2	900	603	0.04%	0.005%
33	5.510	1387	1390	1392	rVB2	583	305	0.02%	0.002%
34	5.526	1392	1395	1397	rBV	421	294	0.02%	0.002%
35	5.561	1401	1406	1409	rBV2	619	584	0.03%	0.005%
36	5.622	1412	1425	1450	rBV	505066	1002353	59.75%	7.768%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041421\
 Data File : VW021012.D
 Acq On : 14 Apr 2021 17:47
 Operator : SY/MD
 Sample : M2031-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG528

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	5.886	1503	1507	1509	rBV2	563	419	0.02%	0.003%
38	6.014	1544	1547	1549	rBV2	890	473	0.03%	0.004%
39	6.072	1552	1565	1586	rBV	356455	715811	42.67%	5.548%
40	6.294	1630	1634	1635	rBV	515	300	0.02%	0.002%
41	6.346	1645	1650	1654	rBV	701	647	0.04%	0.005%
42	6.500	1693	1698	1700	rBV2	550	409	0.02%	0.003%
43	6.580	1721	1723	1728	rVB	542	396	0.02%	0.003%
44	6.612	1729	1733	1735	rBV2	591	471	0.03%	0.004%
45	6.638	1738	1741	1744	rBV3	645	457	0.03%	0.004%
46	6.702	1758	1761	1764	rBV2	489	352	0.02%	0.003%
47	6.744	1772	1774	1776	rBV2	573	264	0.02%	0.002%
48	6.866	1807	1812	1815	rBV	384	463	0.03%	0.004%
49	6.989	1837	1850	1870	rBV2	208304	387571	23.10%	3.004%
50	7.220	1916	1922	1926	rVB3	826	872	0.05%	0.007%
51	7.249	1926	1931	1935	rBV5	923	1127	0.07%	0.009%
52	7.320	1941	1953	1970	rBV	792184	1381320	82.34%	10.705%
53	7.526	2015	2017	2023	rVB4	761	582	0.03%	0.005%
54	7.625	2038	2048	2074	rBV	151060	265739	15.84%	2.060%
55	7.860	2114	2121	2122	rBV4	1702	1884	0.11%	0.015%
56	7.940	2137	2146	2149	rBV2	5908	7405	0.44%	0.057%
57	8.095	2182	2194	2223	rBV	447463	800266	47.70%	6.202%
58	8.616	2354	2356	2358	rBV	480	288	0.02%	0.002%
59	8.857	2418	2431	2453	rBV	748107	1212187	72.26%	9.395%
60	9.153	2515	2523	2531	rBV4	2636	4150	0.25%	0.032%
61	9.307	2566	2571	2572	rBV2	338	291	0.02%	0.002%
62	9.471	2618	2622	2627	rBV2	508	399	0.02%	0.003%
63	9.503	2630	2632	2636	rVB2	698	345	0.02%	0.003%
64	9.558	2642	2649	2656	rBV5	1894	3101	0.18%	0.024%
65	9.641	2672	2675	2678	rVB3	786	460	0.03%	0.004%
66	9.657	2678	2680	2686	rBV2	433	389	0.02%	0.003%
67	9.686	2686	2689	2692	rBV2	517	447	0.03%	0.003%
68	9.812	2722	2728	2730	rBV2	385	342	0.02%	0.003%
69	9.831	2730	2734	2736	rBV2	476	326	0.02%	0.003%
70	9.879	2744	2749	2751	rBV	339	382	0.02%	0.003%
71	9.915	2757	2760	2763	rBV2	381	268	0.02%	0.002%
72	9.937	2763	2767	2772	rVV4	846	749	0.04%	0.006%
73	10.133	2820	2828	2835	rVV6	3847	5393	0.32%	0.042%
74	10.220	2843	2855	2878	rBV	587807	925428	55.17%	7.172%
75	10.355	2894	2897	2898	rBV	687	312	0.02%	0.002%
76	10.580	2965	2967	2970	rBV3	938	491	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021012.D
 Acq On : 14 Apr 2021 17:47
 Operator : SY/MD
 Sample : M2031-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG528

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.834	3041	3046	3050	rBV2	609	730	0.04%	0.006%
78	10.853	3050	3052	3054	rBV2	694	424	0.03%	0.003%
79	10.921	3067	3073	3090	rVB8	5154	8485	0.51%	0.066%
80	11.017	3099	3103	3104	rBV	495	277	0.02%	0.002%
81	11.152	3140	3145	3148	rBV3	1830	1693	0.10%	0.013%
82	11.255	3165	3177	3196	rBV	721689	1128668	67.28%	8.747%
83	11.506	3252	3255	3258	rBV4	1171	1092	0.07%	0.008%
84	11.587	3278	3280	3282	rBV	837	416	0.02%	0.003%
85	11.632	3282	3294	3318	rVV	854212	1336879	79.69%	10.361%
86	11.776	3336	3339	3341	rBV2	1049	689	0.04%	0.005%
87	11.898	3375	3377	3380	rVB2	620	319	0.02%	0.002%
88	11.979	3398	3402	3404	rBV2	647	499	0.03%	0.004%
89	12.123	3444	3447	3450	rVB3	533	337	0.02%	0.003%
90	12.217	3473	3476	3481	rBV	361	292	0.02%	0.002%
91	12.255	3483	3488	3489	rBV2	1229	934	0.06%	0.007%
92	12.429	3538	3542	3547	rBV3	583	563	0.03%	0.004%
93	12.603	3593	3596	3602	rVB3	1013	667	0.04%	0.005%
94	12.657	3607	3613	3620	rBV6	2279	2566	0.15%	0.020%
95	12.812	3658	3661	3663	rBV2	581	397	0.02%	0.003%
96	13.265	3798	3802	3804	rBV2	1316	1042	0.06%	0.008%
97	13.879	3991	3993	3995	rBV2	632	381	0.02%	0.003%
98	13.921	4004	4006	4008	rBV2	765	443	0.03%	0.003%
99	13.966	4018	4020	4023	rBV2	509	320	0.02%	0.002%
100	14.622	4219	4224	4227	rBV3	1219	1100	0.07%	0.009%




Sum of corrected areas: 12903072

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021012.D
Acq On : 14 Apr 2021 17:47
Operator : SY/MD
Sample : M2031-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG528

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

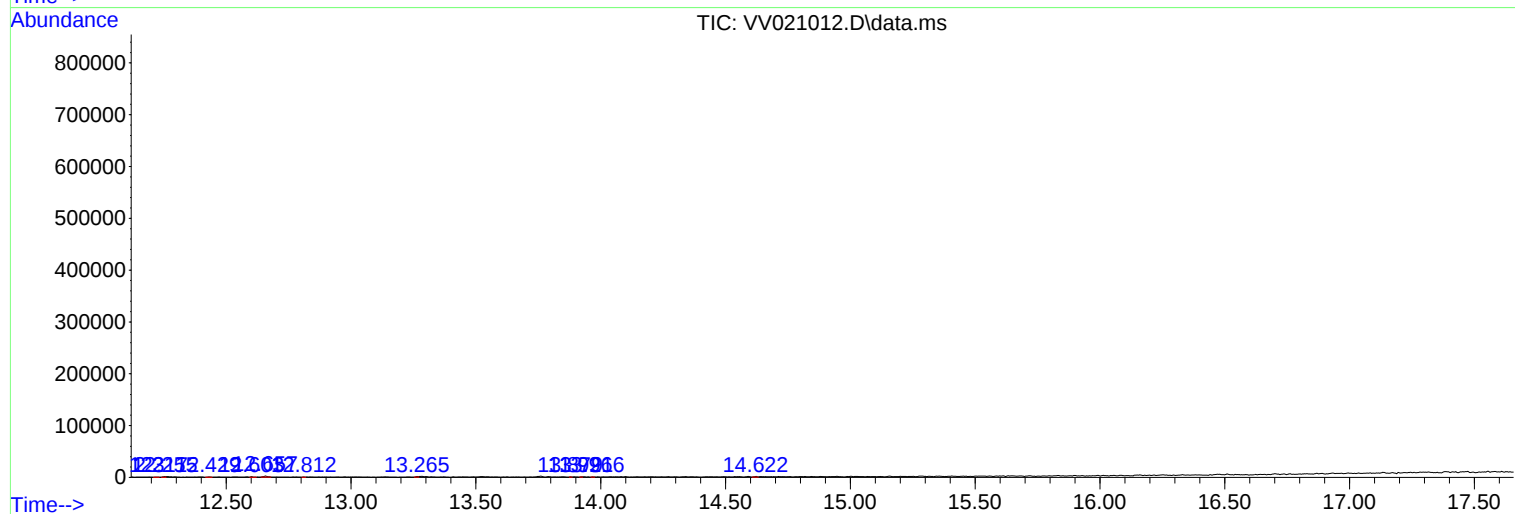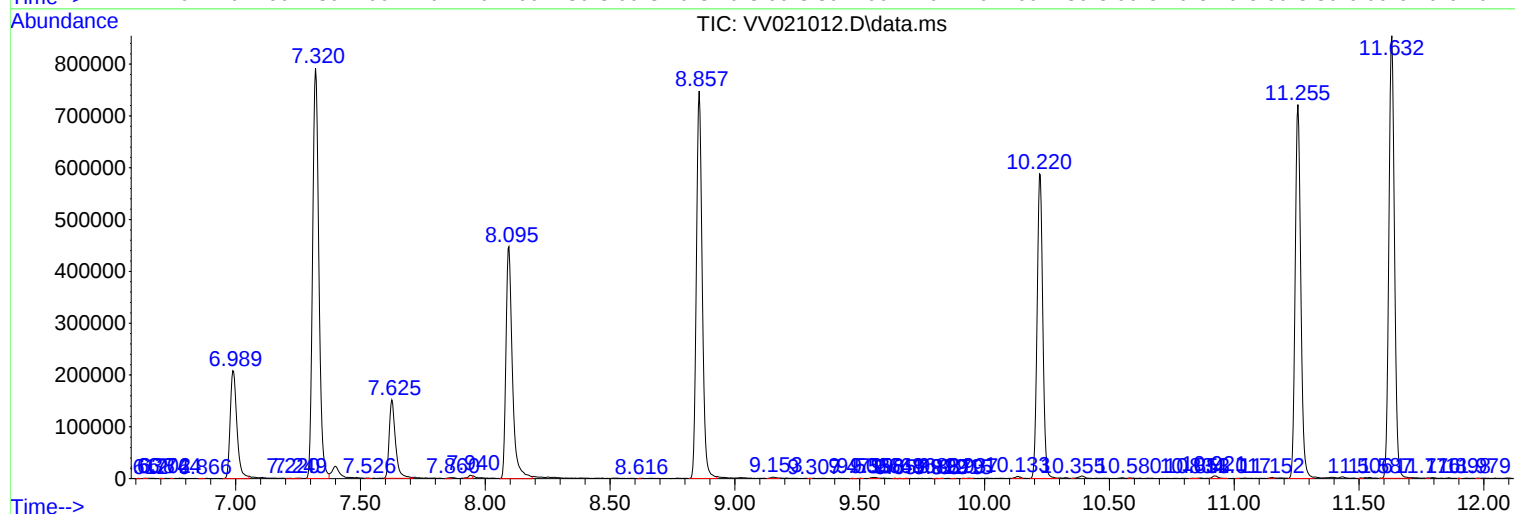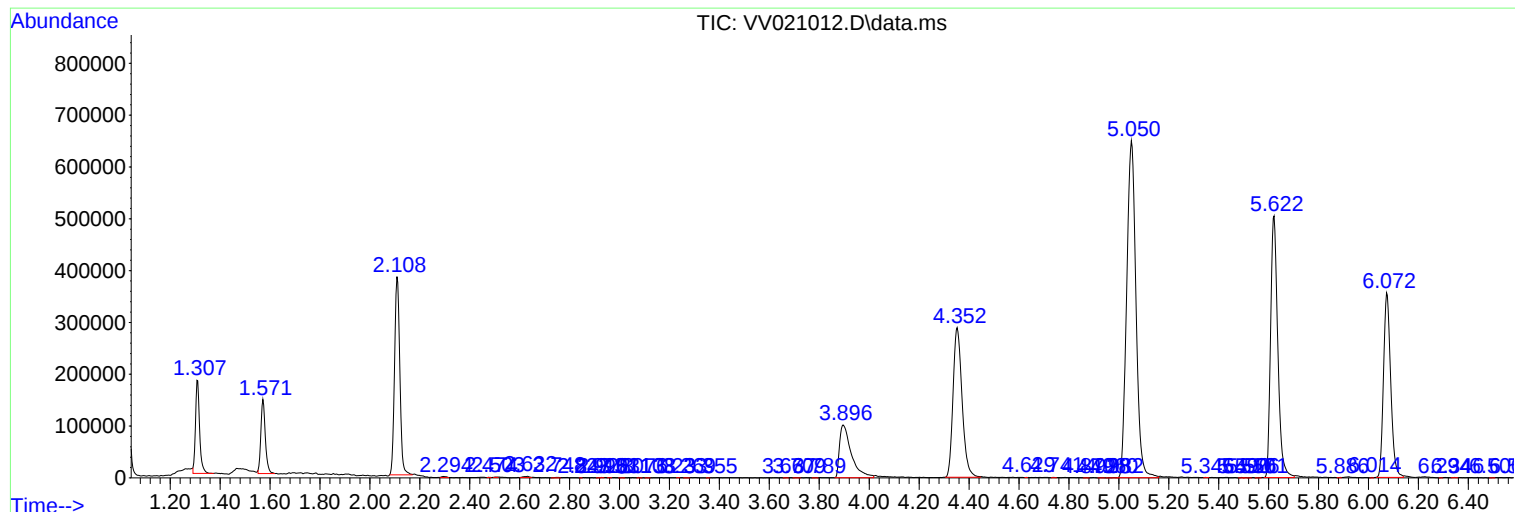

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021012.D
Acq On : 14 Apr 2021 17:47
Operator : SY/MD
Sample : M2031-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG528

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021012.D
Acq On : 14 Apr 2021 17:47
Operator : SY/MD
Sample : M2031-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG528

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
