

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021014.D
 Acq On : 14 Apr 2021 18:34
 Operator : SY/MD
 Sample : M2031-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG536

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

Signal : TIC: VV021014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	78	84	98	rVB	192335	209515	12.08%	1.577%
2	1.571	159	165	181	rVB	154900	189479	10.92%	1.427%
3	2.111	323	333	353	rVB	399542	586561	33.82%	4.416%
4	2.259	377	379	382	rBV2	574	328	0.02%	0.002%
5	2.372	411	414	417	rBV3	465	392	0.02%	0.003%
6	2.452	437	439	440	rBV2	596	286	0.02%	0.002%
7	2.548	466	469	472	rVB2	479	268	0.02%	0.002%
8	2.587	478	481	483	rBV2	400	229	0.01%	0.002%
9	2.632	486	495	502	rVV7	1261	2110	0.12%	0.016%
10	2.693	509	514	518	rBB2	559	501	0.03%	0.004%
11	2.732	518	526	529	rBV3	577	847	0.05%	0.006%
12	2.780	539	541	544	rBV	312	244	0.01%	0.002%
13	3.002	606	610	615	rBV2	569	712	0.04%	0.005%
14	3.044	619	623	624	rBV	320	263	0.02%	0.002%
15	3.089	633	637	639	rBV2	489	455	0.03%	0.003%
16	3.326	707	711	713	rVV	408	278	0.02%	0.002%
17	3.352	716	719	724	rVB2	451	378	0.02%	0.003%
18	3.384	725	729	733	rBV	455	493	0.03%	0.004%
19	3.423	736	741	744	rBV2	621	499	0.03%	0.004%
20	3.526	769	773	775	rBV2	428	298	0.02%	0.002%
21	3.542	775	778	783	rVB2	427	384	0.02%	0.003%
22	3.568	783	786	789	rBV2	595	423	0.02%	0.003%
23	3.651	809	812	814	rBV2	363	239	0.01%	0.002%
24	3.751	838	843	844	rBV2	367	253	0.01%	0.002%
25	3.761	844	846	853	rBV2	473	440	0.03%	0.003%
26	3.809	857	861	864	rBV2	456	391	0.02%	0.003%
27	3.896	878	888	933	rBV2	107513	335179	19.33%	2.524%
28	4.352	1014	1030	1057	rBV	300255	757922	43.70%	5.706%
29	4.535	1085	1087	1088	rBV	676	251	0.01%	0.002%
30	4.661	1123	1126	1127	rBV	674	285	0.02%	0.002%
31	4.680	1130	1132	1138	rVB4	614	571	0.03%	0.004%
32	4.754	1150	1155	1156	rBV2	394	304	0.02%	0.002%
33	4.834	1178	1180	1183	rBV	560	304	0.02%	0.002%
34	4.892	1194	1198	1202	rBV2	473	433	0.02%	0.003%
35	4.918	1202	1206	1209	rVB3	491	460	0.03%	0.003%
36	4.941	1209	1213	1216	rBV	450	451	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021014.D
 Acq On : 14 Apr 2021 18:34
 Operator : SY/MD
 Sample : M2031-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG536

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	5.050	1230	1247	1275	rBV2	668088	1734379	100.00%	13.058%
38	5.426	1361	1364	1369	rVB4	769	591	0.03%	0.004%
39	5.535	1396	1398	1402	rVB2	484	302	0.02%	0.002%
40	5.622	1412	1425	1458	rBV	500994	1012967	58.41%	7.626%
41	5.976	1530	1535	1538	rBV2	959	942	0.05%	0.007%
42	6.027	1549	1551	1553	rBV2	770	405	0.02%	0.003%
43	6.076	1553	1566	1592	rVV	363924	747496	43.10%	5.628%
44	6.268	1624	1626	1631	rVB5	1025	588	0.03%	0.004%
45	6.375	1656	1659	1661	rVB3	694	313	0.02%	0.002%
46	6.445	1679	1681	1682	rBV	689	291	0.02%	0.002%
47	6.490	1691	1695	1697	rBV2	486	302	0.02%	0.002%
48	6.600	1723	1729	1736	rBV3	809	1059	0.06%	0.008%
49	6.677	1750	1753	1757	rVB2	493	358	0.02%	0.003%
50	6.828	1797	1800	1802	rBV	442	253	0.01%	0.002%
51	6.850	1805	1807	1810	rVB2	553	244	0.01%	0.002%
52	6.889	1815	1819	1821	rBV3	410	319	0.02%	0.002%
53	6.915	1824	1827	1830	rBV2	368	314	0.02%	0.002%
54	6.989	1840	1850	1877	rBV	216763	401298	23.14%	3.021%
55	7.223	1920	1923	1925	rBV2	353	230	0.01%	0.002%
56	7.320	1941	1953	1971	rBV	828024	1422432	82.01%	10.709%
57	7.625	2038	2048	2067	rBV2	158039	272721	15.72%	2.053%
58	7.850	2115	2118	2122	rBV2	880	975	0.06%	0.007%
59	8.005	2164	2166	2169	rBV3	640	350	0.02%	0.003%
60	8.092	2183	2193	2228	rBV	480968	844271	48.68%	6.356%
61	8.471	2307	2311	2316	rBV3	566	559	0.03%	0.004%
62	8.593	2345	2349	2350	rBV	620	426	0.02%	0.003%
63	8.680	2374	2376	2379	rBV2	311	231	0.01%	0.002%
64	8.857	2419	2431	2459	rBV	765227	1224561	70.61%	9.220%
65	9.149	2516	2522	2529	rBV5	2613	3769	0.22%	0.028%
66	9.481	2622	2625	2628	rBV2	624	466	0.03%	0.004%
67	9.561	2644	2650	2656	rVV4	1707	1981	0.11%	0.015%
68	9.677	2684	2686	2689	rBV	593	381	0.02%	0.003%
69	9.844	2730	2738	2743	rBV5	920	1221	0.07%	0.009%
70	9.944	2767	2769	2771	rBV2	581	289	0.02%	0.002%
71	10.133	2822	2828	2834	rVV4	3530	4031	0.23%	0.030%
72	10.220	2842	2855	2873	rBV	602027	956586	55.15%	7.202%
73	10.352	2893	2896	2897	rBV2	622	269	0.02%	0.002%
74	10.448	2922	2926	2930	rBV3	799	892	0.05%	0.007%
75	10.548	2950	2957	2959	rBV4	668	839	0.05%	0.006%
76	10.927	3065	3075	3081	rBV7	4402	6463	0.37%	0.049%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021014.D
 Acq On : 14 Apr 2021 18:34
 Operator : SY/MD
 Sample : M2031-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG536

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	11.037	3106	3109	3110	rBV2	625	317	0.02%	0.002%
78	11.153	3137	3145	3152	rBV9	1940	3394	0.20%	0.026%
79	11.255	3165	3177	3201	rBV	737218	1136826	65.55%	8.559%
80	11.365	3209	3211	3213	rBV2	821	297	0.02%	0.002%
81	11.632	3282	3294	3319	rVB	878764	1393661	80.36%	10.493%
82	11.783	3337	3341	3343	rBV5	662	545	0.03%	0.004%
83	11.870	3366	3368	3369	rBV5	762	313	0.02%	0.002%
84	11.947	3389	3392	3395	rBV	320	244	0.01%	0.002%
85	12.140	3449	3452	3457	rBV	629	501	0.03%	0.004%
86	12.175	3460	3463	3465	rBV	345	237	0.01%	0.002%
87	12.201	3470	3471	3475	rVB3	575	328	0.02%	0.002%
88	12.435	3542	3544	3547	rBV2	447	311	0.02%	0.002%
89	12.522	3568	3571	3573	rBV3	424	286	0.02%	0.002%
90	12.577	3584	3588	3593	rBV2	676	609	0.04%	0.005%
91	12.599	3593	3595	3598	rBV2	437	260	0.01%	0.002%
92	12.651	3609	3611	3613	rBV2	782	489	0.03%	0.004%
93	13.014	3722	3724	3729	rVB2	758	590	0.03%	0.004%
94	13.107	3749	3753	3756	rBV	450	440	0.03%	0.003%
95	13.323	3818	3820	3825	rVB2	597	417	0.02%	0.003%
96	13.522	3879	3882	3888	rBV3	1161	1339	0.08%	0.010%
97	13.757	3952	3955	3959	rBV3	1184	758	0.04%	0.006%
98	13.972	4020	4022	4023	rBV3	553	276	0.02%	0.002%
99	14.506	4186	4188	4189	rBV	750	247	0.01%	0.002%
100	14.879	4301	4304	4306	rBV	1126	778	0.04%	0.006%




Sum of corrected areas: 13282253

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021014.D
Acq On : 14 Apr 2021 18:34
Operator : SY/MD
Sample : M2031-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG536

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

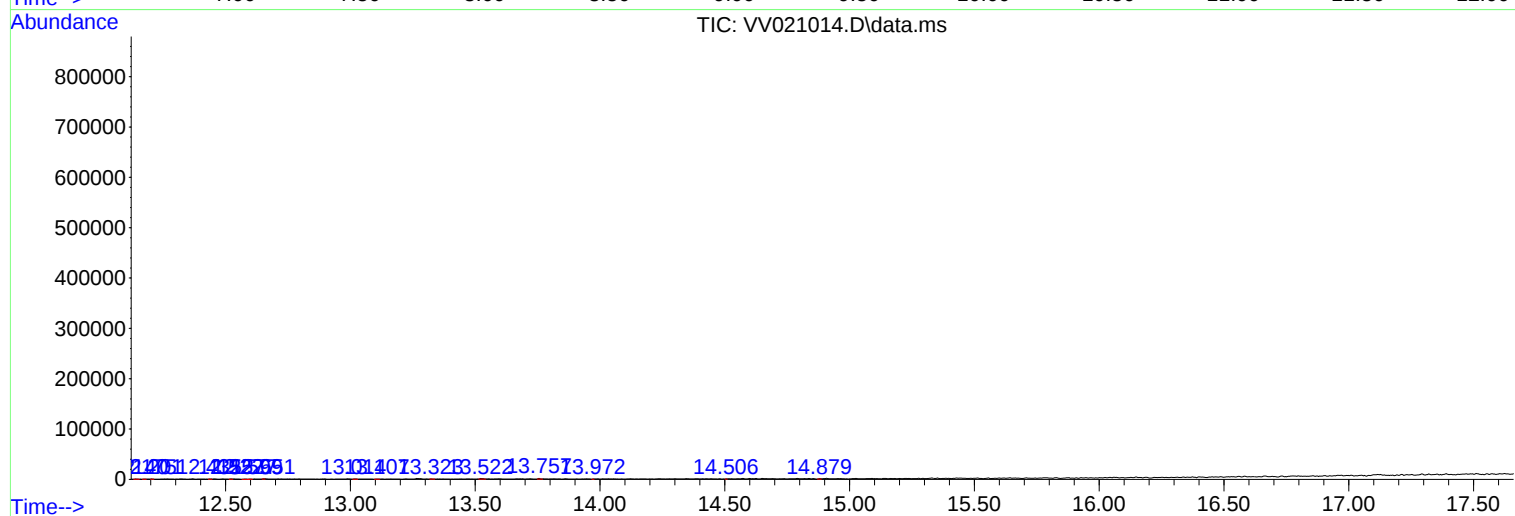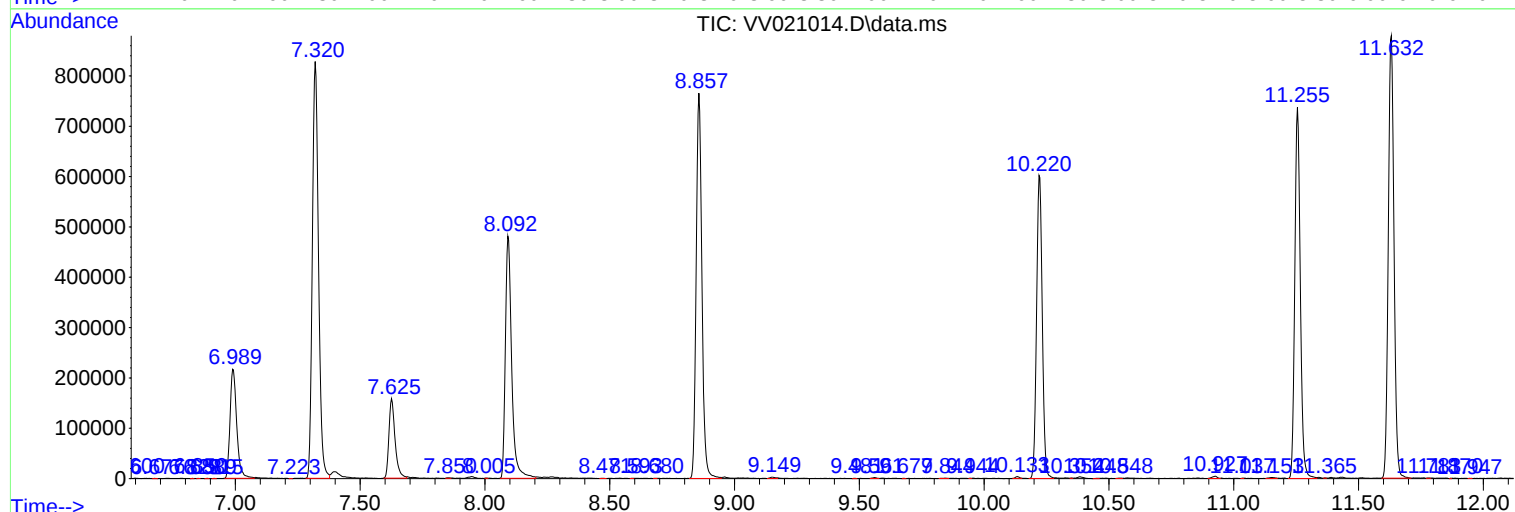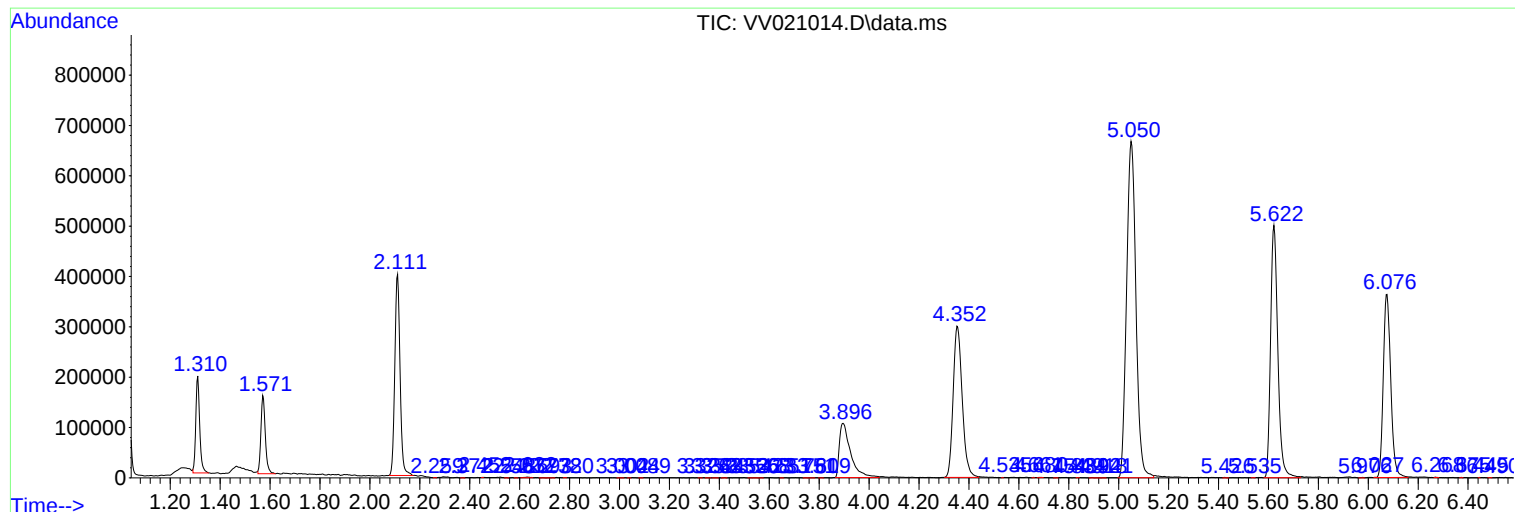

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021014.D
Acq On : 14 Apr 2021 18:34
Operator : SY/MD
Sample : M2031-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG536

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021014.D
Acq On : 14 Apr 2021 18:34
Operator : SY/MD
Sample : M2031-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG536

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
