

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021015.D
 Acq On : 14 Apr 2021 18:57
 Operator : SY/MD
 Sample : M2031-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG537

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M

Title : VOC Analysis

Signal : TIC: VV021015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	78	84	101	rVB	189390	209157	12.36%	1.596%
2	1.571	159	165	177	rVB	151208	183867	10.87%	1.403%
3	2.111	323	333	358	rBV	378870	560641	33.14%	4.277%
4	2.301	383	392	399	rBV2	2366	3753	0.22%	0.029%
5	2.378	410	416	418	rBV2	603	489	0.03%	0.004%
6	2.452	436	439	442	rBV2	807	570	0.03%	0.004%
7	2.516	452	459	465	rBV8	1488	1918	0.11%	0.015%
8	2.584	478	480	482	rBV2	562	295	0.02%	0.002%
9	2.670	505	507	513	rVB2	369	303	0.02%	0.002%
10	2.764	533	536	538	rBV2	685	422	0.02%	0.003%
11	2.802	545	548	550	rBV2	503	317	0.02%	0.002%
12	2.857	563	565	569	rBV2	462	334	0.02%	0.003%
13	2.963	595	598	600	rBV	443	333	0.02%	0.003%
14	3.214	674	676	679	rBV	540	358	0.02%	0.003%
15	3.307	702	705	706	rBV	399	269	0.02%	0.002%
16	3.506	764	767	769	rBV	549	291	0.02%	0.002%
17	3.683	818	822	825	rBV2	478	408	0.02%	0.003%
18	3.735	836	838	843	rVB	466	354	0.02%	0.003%
19	3.776	847	851	853	rVB	310	232	0.01%	0.002%
20	3.796	854	857	863	rBB	622	511	0.03%	0.004%
21	3.895	878	888	921	rBV2	102259	326668	19.31%	2.492%
22	4.355	1012	1031	1061	rBV2	293760	739674	43.72%	5.643%
23	4.580	1099	1101	1103	rBV2	620	294	0.02%	0.002%
24	4.767	1156	1159	1161	rBV3	646	407	0.02%	0.003%
25	4.886	1191	1196	1198	rBV2	472	360	0.02%	0.003%
26	4.947	1210	1215	1218	rBV3	335	338	0.02%	0.003%
27	4.966	1218	1221	1223	rBV2	532	319	0.02%	0.002%
28	5.050	1229	1247	1274	rBV2	650419	1691815	100.00%	12.906%
29	5.391	1349	1353	1359	rVB4	927	1072	0.06%	0.008%
30	5.426	1359	1364	1365	rBV	873	533	0.03%	0.004%
31	5.468	1372	1377	1378	rBV	331	252	0.01%	0.002%
32	5.503	1384	1388	1392	rBV3	680	600	0.04%	0.005%
33	5.526	1392	1395	1396	rBV2	534	275	0.02%	0.002%
34	5.622	1413	1425	1451	rBV	510679	1016579	60.09%	7.755%
35	5.918	1512	1517	1524	rBV7	1588	2273	0.13%	0.017%
36	6.075	1552	1566	1588	rBV2	358576	730813	43.20%	5.575%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021015.D
 Acq On : 14 Apr 2021 18:57
 Operator : SY/MD
 Sample : M2031-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG537

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.326	1641	1644	1648	rBV4	703	539	0.03%	0.004%
38	6.403	1666	1668	1671	rBV3	519	266	0.02%	0.002%
39	6.442	1678	1680	1682	rBV	638	347	0.02%	0.003%
40	6.503	1693	1699	1701	rBV3	673	694	0.04%	0.005%
41	6.529	1705	1707	1711	rVV2	426	306	0.02%	0.002%
42	6.616	1731	1734	1736	rBV	483	267	0.02%	0.002%
43	6.677	1749	1753	1756	rBV2	344	378	0.02%	0.003%
44	6.715	1762	1765	1769	rVB2	599	482	0.03%	0.004%
45	6.751	1770	1776	1777	rBV3	475	387	0.02%	0.003%
46	6.886	1813	1818	1823	rBV	649	653	0.04%	0.005%
47	6.915	1823	1827	1830	rBV3	409	342	0.02%	0.003%
48	6.989	1836	1850	1869	rBV	209294	387467	22.90%	2.956%
49	7.230	1920	1925	1930	rBV3	929	1149	0.07%	0.009%
50	7.320	1941	1953	1972	rBV	804635	1395924	82.51%	10.649%
51	7.625	2038	2048	2073	rBV	154841	272030	16.08%	2.075%
52	7.857	2114	2120	2123	rBV5	2140	2372	0.14%	0.018%
53	7.934	2137	2144	2145	rBV3	2803	2298	0.14%	0.018%
54	7.979	2156	2158	2162	rBV3	1225	674	0.04%	0.005%
55	8.091	2182	2193	2220	rBV	470840	821019	48.53%	6.263%
56	8.416	2293	2294	2297	rBV	627	321	0.02%	0.002%
57	8.474	2310	2312	2314	rBV2	529	257	0.02%	0.002%
58	8.532	2328	2330	2334	rBV2	393	345	0.02%	0.003%
59	8.558	2334	2338	2341	rBV2	639	460	0.03%	0.004%
60	8.644	2362	2365	2366	rBV	488	273	0.02%	0.002%
61	8.677	2372	2375	2381	rVB2	574	417	0.02%	0.003%
62	8.812	2415	2417	2419	rBV2	578	266	0.02%	0.002%
63	8.857	2419	2431	2456	rBV	767144	1247174	73.72%	9.514%
64	9.146	2518	2521	2522	rBV	972	496	0.03%	0.004%
65	9.345	2581	2583	2585	rBV	738	348	0.02%	0.003%
66	9.429	2607	2609	2612	rBV2	409	255	0.02%	0.002%
67	9.477	2622	2624	2628	rBV	407	265	0.02%	0.002%
68	9.516	2632	2636	2639	rBV2	391	362	0.02%	0.003%
69	9.683	2684	2688	2692	rBV2	421	371	0.02%	0.003%
70	9.731	2700	2703	2706	rVB	825	473	0.03%	0.004%
71	9.815	2728	2729	2732	rVB2	550	260	0.02%	0.002%
72	9.937	2763	2767	2771	rVB3	645	503	0.03%	0.004%
73	9.988	2779	2783	2785	rBV2	401	266	0.02%	0.002%
74	10.043	2798	2800	2803	rVB2	479	311	0.02%	0.002%
75	10.133	2820	2828	2837	rVB6	3849	5869	0.35%	0.045%
76	10.223	2843	2856	2875	rBV	605654	940530	55.59%	7.175%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021015.D
 Acq On : 14 Apr 2021 18:57
 Operator : SY/MD
 Sample : M2031-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG537

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.464	2929	2931	2935	rVB3	674	415	0.02%	0.003%
78	10.577	2962	2966	2969	rBV2	945	749	0.04%	0.006%
79	10.644	2981	2987	2989	rBV2	444	498	0.03%	0.004%
80	10.789	3029	3032	3034	rBV3	544	319	0.02%	0.002%
81	10.924	3066	3074	3081	rVB7	4191	6139	0.36%	0.047%
82	11.043	3107	3111	3114	rVB2	598	566	0.03%	0.004%
83	11.255	3166	3177	3198	rBV	752441	1155739	68.31%	8.817%
84	11.435	3228	3233	3243	rVB7	2467	3654	0.22%	0.028%
85	11.631	3282	3294	3316	rBV	882022	1366942	80.80%	10.428%
86	11.789	3340	3343	3351	rVB6	2073	2327	0.14%	0.018%
87	11.821	3351	3353	3356	rBV3	523	299	0.02%	0.002%
88	11.850	3359	3362	3363	rBV2	903	534	0.03%	0.004%
89	12.008	3407	3411	3412	rBV	601	319	0.02%	0.002%
90	12.059	3424	3427	3429	rBV2	598	281	0.02%	0.002%
91	12.168	3459	3461	3463	rBV	681	319	0.02%	0.002%
92	12.525	3569	3572	3576	rBV3	657	493	0.03%	0.004%
93	12.596	3590	3594	3596	rBV3	1874	1373	0.08%	0.010%
94	12.638	3603	3607	3609	rBV2	705	565	0.03%	0.004%
95	12.889	3683	3685	3688	rBV3	667	386	0.02%	0.003%
96	13.348	3826	3828	3831	rBV2	566	340	0.02%	0.003%
97	13.509	3876	3878	3881	rBV	754	303	0.02%	0.002%
98	13.528	3881	3884	3887	rVV2	743	531	0.03%	0.004%
99	13.937	4009	4011	4012	rBV	630	322	0.02%	0.002%
100	14.435	4163	4166	4169	rBV2	1045	765	0.05%	0.006%




Sum of corrected areas: 13108688

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021015.D
Acq On : 14 Apr 2021 18:57
Operator : SY/MD
Sample : M2031-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG537

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

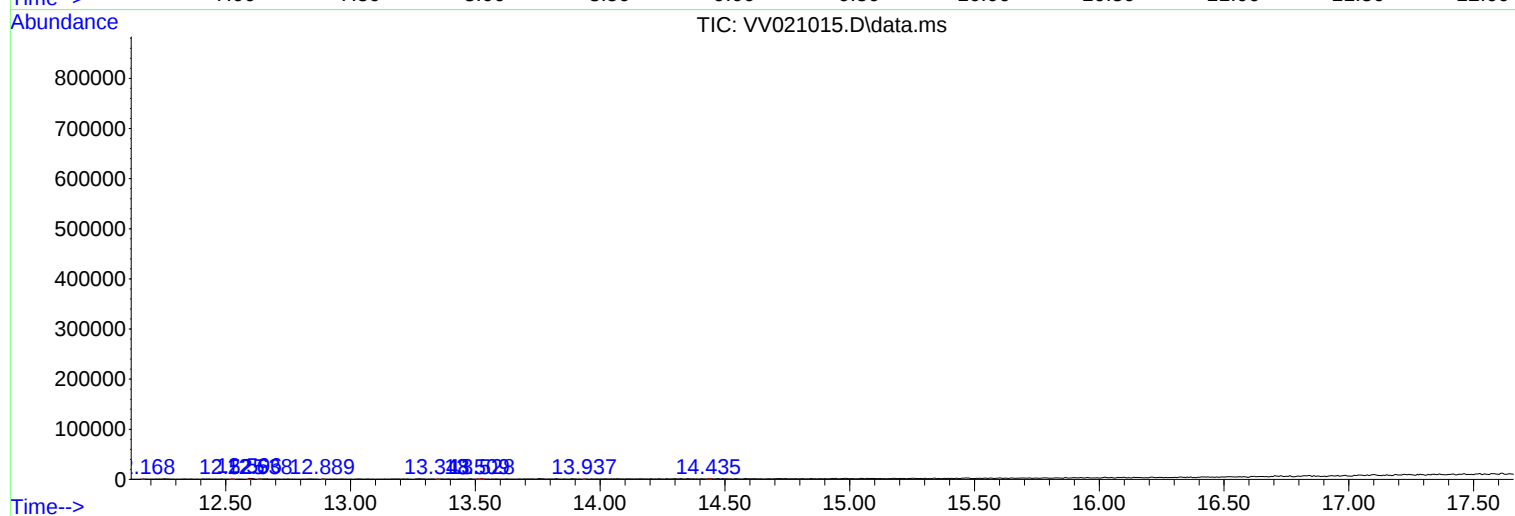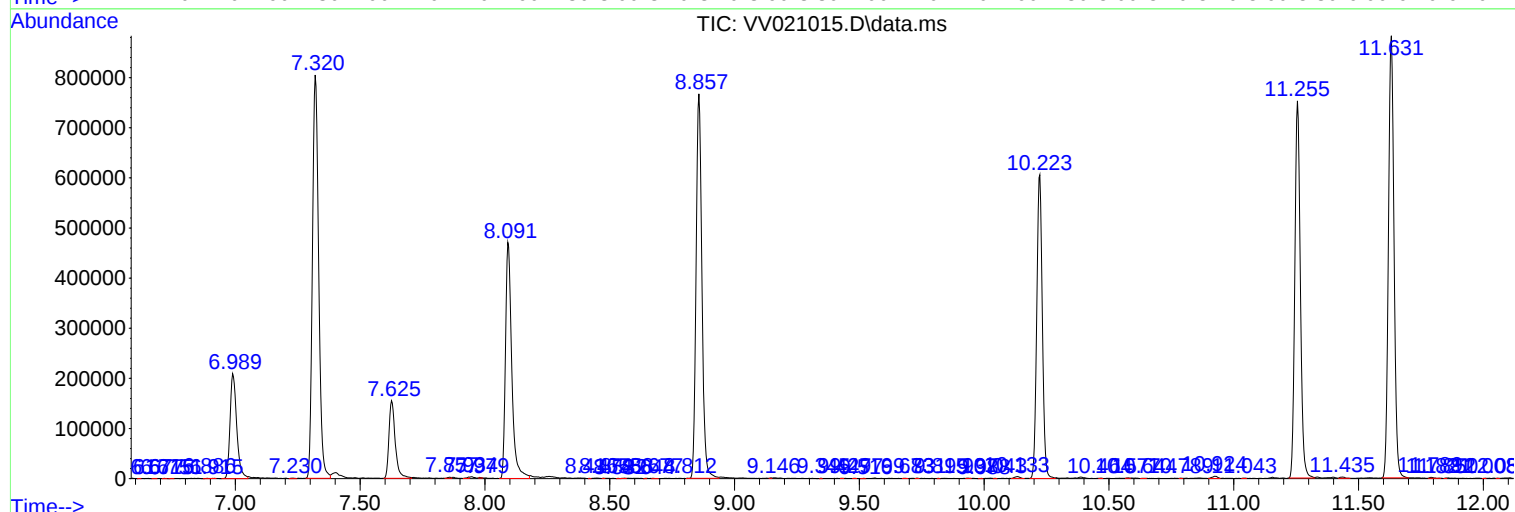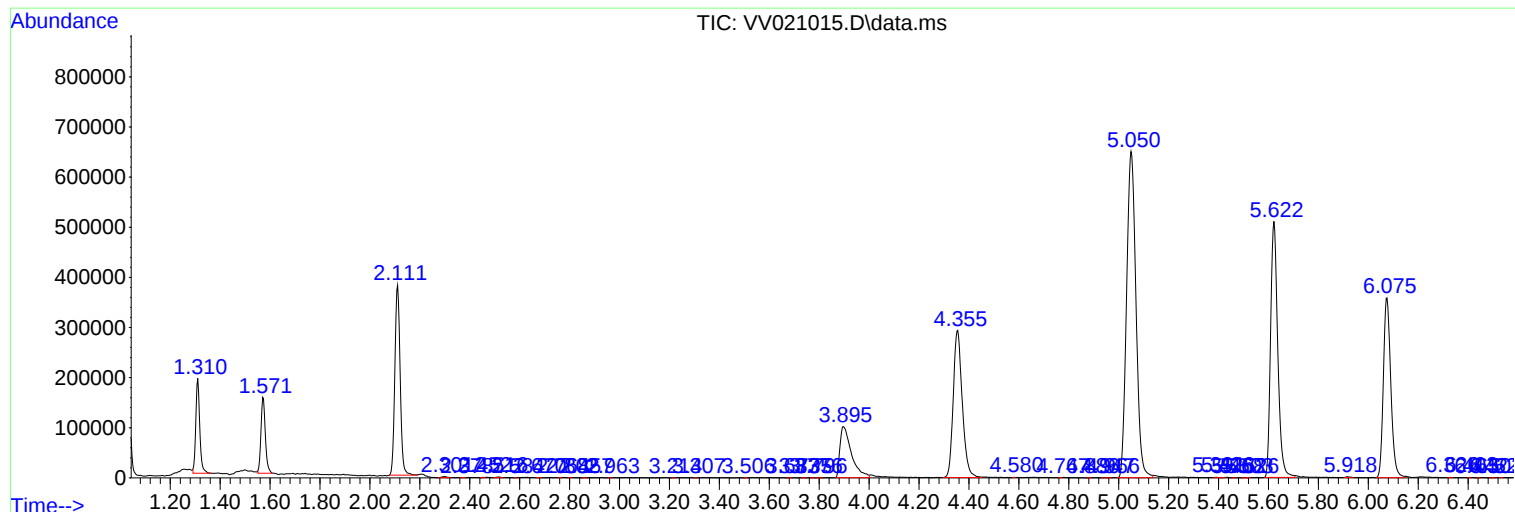

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021015.D
Acq On : 14 Apr 2021 18:57
Operator : SY/MD
Sample : M2031-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG537

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021015.D
Acq On : 14 Apr 2021 18:57
Operator : SY/MD
Sample : M2031-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG537

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
