

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021016.D
 Acq On : 14 Apr 2021 19:21
 Operator : SY/MD
 Sample : M2031-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG538

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

Signal : TIC: VV021016.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	78	84	98	rVB	187895	210649	12.19%	1.554%
2	1.571	159	165	181	rVB	157913	196505	11.37%	1.450%
3	2.108	322	332	347	rBV	395601	574597	33.25%	4.240%
4	2.384	415	418	421	rBV2	461	231	0.01%	0.002%
5	2.401	421	423	425	rBV	421	231	0.01%	0.002%
6	2.410	425	426	430	rVB	685	400	0.02%	0.003%
7	2.446	430	437	439	rBV3	917	1138	0.07%	0.008%
8	2.687	507	512	515	rBV2	491	374	0.02%	0.003%
9	2.741	527	529	532	rVV2	442	248	0.01%	0.002%
10	2.783	535	542	548	rVB4	992	1185	0.07%	0.009%
11	2.873	568	570	576	rVB2	388	259	0.01%	0.002%
12	2.905	578	580	585	rVB2	508	399	0.02%	0.003%
13	2.931	585	588	591	rBV	483	404	0.02%	0.003%
14	2.960	595	597	600	rVB2	380	232	0.01%	0.002%
15	2.989	602	606	609	rBV	594	596	0.03%	0.004%
16	3.121	644	647	648	rBV	461	286	0.02%	0.002%
17	3.237	678	683	685	rVB2	490	377	0.02%	0.003%
18	3.253	685	688	690	rBV	654	275	0.02%	0.002%
19	3.265	690	692	698	rVB2	601	548	0.03%	0.004%
20	3.317	704	708	712	rBV	617	577	0.03%	0.004%
21	3.568	782	786	788	rVV	306	222	0.01%	0.002%
22	3.593	791	794	797	rVB2	495	326	0.02%	0.002%
23	3.619	800	802	807	rVB2	378	248	0.01%	0.002%
24	3.722	832	834	837	rBV2	341	212	0.01%	0.002%
25	3.905	877	891	918	rBV	102225	341595	19.77%	2.520%
26	4.220	987	989	993	rVB	1052	518	0.03%	0.004%
27	4.352	1013	1030	1060	rBV2	305055	768972	44.49%	5.674%
28	4.600	1104	1107	1108	rBV	589	349	0.02%	0.003%
29	4.735	1147	1149	1152	rBV2	519	229	0.01%	0.002%
30	4.905	1200	1202	1206	rBV	441	362	0.02%	0.003%
31	4.931	1206	1210	1213	rBV2	606	555	0.03%	0.004%
32	5.050	1227	1247	1279	rBV2	672351	1728259	100.00%	12.752%
33	5.346	1337	1339	1342	rBV	830	460	0.03%	0.003%
34	5.371	1342	1347	1349	rVV4	992	810	0.05%	0.006%
35	5.622	1411	1425	1453	rBV	543459	1084863	62.77%	8.005%
36	5.757	1465	1467	1471	rBV3	1185	875	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021016.D
 Acq On : 14 Apr 2021 19:21
 Operator : SY/MD
 Sample : M2031-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG538

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	5.915	1508	1516	1518	rBV6	1958	2617	0.15%	0.019%
38	6.005	1540	1544	1545	rBV	436	331	0.02%	0.002%
39	6.072	1552	1565	1589	rBV2	366050	748684	43.32%	5.524%
40	6.323	1641	1643	1647	rVV4	792	452	0.03%	0.003%
41	6.349	1649	1651	1654	rVB	613	307	0.02%	0.002%
42	6.494	1692	1696	1697	rBV2	640	475	0.03%	0.004%
43	6.545	1708	1712	1716	rBV2	741	728	0.04%	0.005%
44	6.609	1729	1732	1736	rVB3	578	321	0.02%	0.002%
45	6.677	1747	1753	1754	rBV2	621	445	0.03%	0.003%
46	6.703	1758	1761	1763	rBV2	559	364	0.02%	0.003%
47	6.741	1772	1773	1776	rBV	381	247	0.01%	0.002%
48	6.796	1786	1790	1792	rBV	304	236	0.01%	0.002%
49	6.992	1837	1851	1872	rBV	214790	398884	23.08%	2.943%
50	7.159	1900	1903	1904	rBV2	708	454	0.03%	0.003%
51	7.211	1917	1919	1925	rBV4	734	493	0.03%	0.004%
52	7.240	1925	1928	1931	rBV3	762	531	0.03%	0.004%
53	7.320	1941	1953	1970	rBV	818833	1403801	81.23%	10.358%
54	7.625	2037	2048	2072	rBV	155939	274800	15.90%	2.028%
55	7.941	2142	2146	2154	rBV3	2571	2855	0.17%	0.021%
56	8.024	2169	2172	2174	rBV	469	246	0.01%	0.002%
57	8.037	2174	2176	2179	rVB2	555	326	0.02%	0.002%
58	8.095	2181	2194	2227	rBV	492579	881696	51.02%	6.506%
59	8.690	2376	2379	2380	rBV2	581	348	0.02%	0.003%
60	8.780	2405	2407	2411	rVB2	578	323	0.02%	0.002%
61	8.857	2418	2431	2453	rBV	815609	1308720	75.72%	9.656%
62	9.124	2513	2514	2518	rBV2	453	304	0.02%	0.002%
63	9.153	2519	2523	2525	rBV3	1142	1086	0.06%	0.008%
64	9.285	2562	2564	2566	rVB2	655	273	0.02%	0.002%
65	9.301	2566	2569	2572	rBV2	701	436	0.03%	0.003%
66	9.330	2576	2578	2581	rBV	315	220	0.01%	0.002%
67	9.387	2591	2596	2603	rBV2	370	397	0.02%	0.003%
68	9.500	2628	2631	2633	rBV2	473	244	0.01%	0.002%
69	9.712	2693	2697	2701	rBV	671	550	0.03%	0.004%
70	9.805	2722	2726	2730	rBV	480	399	0.02%	0.003%
71	9.883	2748	2750	2754	rVB2	626	387	0.02%	0.003%
72	9.937	2765	2767	2769	rBV	457	288	0.02%	0.002%
73	9.979	2776	2780	2784	rBV3	533	485	0.03%	0.004%
74	10.011	2787	2790	2797	rVV	867	584	0.03%	0.004%
75	10.059	2801	2805	2808	rVB2	535	399	0.02%	0.003%
76	10.133	2822	2828	2836	rVB3	4082	5704	0.33%	0.042%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021016.D
 Acq On : 14 Apr 2021 19:21
 Operator : SY/MD
 Sample : M2031-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG538

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.172	2838	2840	2842	rBV2	489	233	0.01%	0.002%
78	10.220	2844	2855	2875	rBV	625574	963770	55.77%	7.111%
79	10.326	2885	2888	2891	rBV2	683	443	0.03%	0.003%
80	10.767	3021	3025	3028	rBV2	628	483	0.03%	0.004%
81	10.924	3068	3074	3086	rVB6	4892	7237	0.42%	0.053%
82	11.153	3138	3145	3151	rBV6	1567	2514	0.15%	0.019%
83	11.256	3164	3177	3196	rBV	789486	1216665	70.40%	8.977%
84	11.548	3266	3268	3273	rVB2	1042	531	0.03%	0.004%
85	11.632	3281	3294	3310	rBV	892895	1394060	80.66%	10.286%
86	11.854	3361	3363	3366	rBV3	723	523	0.03%	0.004%
87	12.030	3416	3418	3423	rVB4	631	402	0.02%	0.003%
88	12.101	3436	3440	3441	rBV3	709	480	0.03%	0.004%
89	12.362	3517	3521	3525	rBV3	626	594	0.03%	0.004%
90	12.493	3559	3562	3565	rBV3	845	667	0.04%	0.005%
91	12.593	3590	3593	3594	rBV2	889	545	0.03%	0.004%
92	12.690	3618	3623	3626	rVB3	733	639	0.04%	0.005%
93	12.718	3626	3632	3633	rBV2	868	776	0.04%	0.006%
94	13.030	3726	3729	3732	rBV3	678	539	0.03%	0.004%
95	13.198	3779	3781	3785	rVB2	605	310	0.02%	0.002%
96	13.281	3800	3807	3808	rBV3	896	890	0.05%	0.007%
97	13.593	3903	3904	3906	rBV	405	222	0.01%	0.002%
98	13.898	3996	3999	4003	rBV3	761	598	0.03%	0.004%
99	14.361	4141	4143	4147	rBV3	709	437	0.03%	0.003%
100	15.008	4341	4344	4345	rBV2	1310	670	0.04%	0.005%


Sum of corrected areas: 13553034

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021016.D
Acq On : 14 Apr 2021 19:21
Operator : SY/MD
Sample : M2031-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG538

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

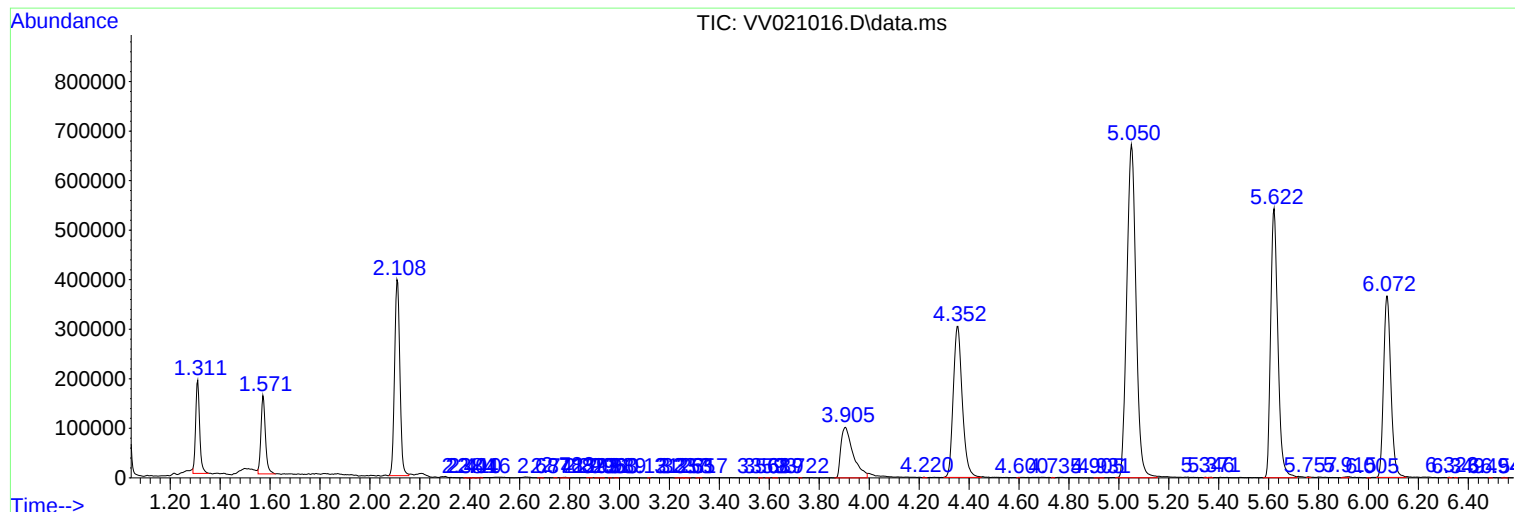

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021016.D
Acq On : 14 Apr 2021 19:21
Operator : SY/MD
Sample : M2031-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG538

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021016.D
Acq On : 14 Apr 2021 19:21
Operator : SY/MD
Sample : M2031-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG538

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
