

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021017.D
 Acq On : 14 Apr 2021 19:44
 Operator : SY/MD
 Sample : M2031-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG539

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M

Title : VOC Analysis

Signal : TIC: VV021017.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	78	84	98	rVB	179823	203507	11.89%	1.524%
2	1.571	159	165	182	rVB	148883	193147	11.29%	1.446%
3	2.108	323	332	355	rVB	391688	561339	32.80%	4.203%
4	2.609	485	488	491	rBV4	974	778	0.05%	0.006%
5	2.735	524	527	529	rBV	453	259	0.02%	0.002%
6	2.777	536	540	544	rVB3	486	408	0.02%	0.003%
7	2.883	571	573	577	rBV2	338	258	0.02%	0.002%
8	2.908	579	581	584	rVB3	506	244	0.01%	0.002%
9	2.976	600	602	608	rVB	593	560	0.03%	0.004%
10	3.021	613	616	617	rBV	504	241	0.01%	0.002%
11	3.037	619	621	628	rVB	574	394	0.02%	0.003%
12	3.088	634	637	640	rVB2	464	322	0.02%	0.002%
13	3.140	646	653	657	rBV2	466	647	0.04%	0.005%
14	3.278	694	696	699	rVB	661	367	0.02%	0.003%
15	3.426	740	742	744	rBV2	422	290	0.02%	0.002%
16	3.465	750	754	756	rBV2	421	386	0.02%	0.003%
17	3.577	785	789	793	rBV2	449	479	0.03%	0.004%
18	3.622	800	803	806	rBV	343	234	0.01%	0.002%
19	3.773	846	850	852	rBV2	636	453	0.03%	0.003%
20	3.786	852	854	859	rBV2	454	274	0.02%	0.002%
21	3.828	864	867	868	rBV	395	227	0.01%	0.002%
22	3.908	880	892	929	rBV2	95338	349589	20.43%	2.617%
23	4.352	1015	1030	1060	rBV	295686	748463	43.74%	5.604%
24	4.632	1114	1117	1120	rBV3	628	393	0.02%	0.003%
25	4.657	1122	1125	1127	rBV2	559	359	0.02%	0.003%
26	4.818	1173	1175	1179	rBV3	528	335	0.02%	0.003%
27	4.841	1179	1182	1185	rBV3	588	350	0.02%	0.003%
28	4.931	1206	1210	1214	rBV3	593	523	0.03%	0.004%
29	4.953	1214	1217	1220	rBV	634	454	0.03%	0.003%
30	5.050	1230	1247	1280	rBV2	667211	1711221	100.00%	12.811%
31	5.329	1330	1334	1337	rBV3	1172	922	0.05%	0.007%
32	5.439	1366	1368	1371	rBV2	422	314	0.02%	0.002%
33	5.500	1383	1387	1391	rBV2	512	468	0.03%	0.004%
34	5.551	1401	1403	1409	rVB2	433	349	0.02%	0.003%
35	5.622	1412	1425	1454	rBV	527157	1061885	62.05%	7.950%
36	5.956	1526	1529	1530	rBV2	458	224	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021017.D
 Acq On : 14 Apr 2021 19:44
 Operator : SY/MD
 Sample : M2031-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG539

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	5.989	1536	1539	1544	rBV2	647	540	0.03%	0.004%
38	6.011	1544	1546	1548	rBV2	619	374	0.02%	0.003%
39	6.075	1552	1566	1587	rBV2	364290	739155	43.19%	5.534%
40	6.320	1639	1642	1645	rVB3	588	342	0.02%	0.003%
41	6.345	1645	1650	1651	rBV2	586	306	0.02%	0.002%
42	6.365	1654	1656	1659	rVB	566	312	0.02%	0.002%
43	6.448	1680	1682	1684	rBV3	408	237	0.01%	0.002%
44	6.506	1696	1700	1703	rBV	333	359	0.02%	0.003%
45	6.542	1708	1711	1716	rVV2	876	672	0.04%	0.005%
46	6.561	1716	1717	1725	rVB3	561	454	0.03%	0.003%
47	6.632	1736	1739	1743	rVB2	428	252	0.01%	0.002%
48	6.728	1767	1769	1774	rVB2	391	258	0.02%	0.002%
49	6.989	1839	1850	1871	rBV	219447	395660	23.12%	2.962%
50	7.320	1941	1953	1972	rBV	816227	1400597	81.85%	10.486%
51	7.625	2037	2048	2078	rBV	157753	278709	16.29%	2.087%
52	7.763	2089	2091	2093	rBV2	904	416	0.02%	0.003%
53	7.825	2108	2110	2113	rBV2	414	278	0.02%	0.002%
54	7.857	2113	2120	2122	rBV6	2445	2334	0.14%	0.017%
55	7.947	2137	2148	2156	rBV5	3180	5685	0.33%	0.043%
56	7.982	2156	2159	2165	rVB6	1887	1986	0.12%	0.015%
57	8.095	2184	2194	2231	rBV	482950	868157	50.73%	6.500%
58	8.397	2285	2288	2290	rBV2	455	251	0.01%	0.002%
59	8.538	2330	2332	2334	rBV	456	253	0.01%	0.002%
60	8.596	2346	2350	2352	rBV2	400	255	0.01%	0.002%
61	8.619	2353	2357	2362	rBV2	486	417	0.02%	0.003%
62	8.641	2362	2364	2367	rVB2	523	297	0.02%	0.002%
63	8.661	2367	2370	2374	rBV2	600	579	0.03%	0.004%
64	8.786	2406	2409	2411	rBV2	508	255	0.01%	0.002%
65	8.857	2418	2431	2456	rBV	797516	1284088	75.04%	9.614%
66	9.066	2493	2496	2497	rBV2	549	278	0.02%	0.002%
67	9.152	2515	2523	2525	rBV6	2275	2934	0.17%	0.022%
68	9.246	2548	2552	2557	rBV2	471	452	0.03%	0.003%
69	9.271	2557	2560	2562	rBV2	547	335	0.02%	0.003%
70	9.313	2570	2573	2576	rBV2	365	262	0.02%	0.002%
71	9.480	2622	2625	2628	rBV2	389	303	0.02%	0.002%
72	9.664	2680	2682	2685	rBV	480	268	0.02%	0.002%
73	9.725	2698	2701	2703	rBV	542	405	0.02%	0.003%
74	9.751	2707	2709	2711	rVB	546	223	0.01%	0.002%
75	9.763	2711	2713	2716	rBV	424	296	0.02%	0.002%
76	9.821	2727	2731	2732	rBV	371	256	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021017.D
 Acq On : 14 Apr 2021 19:44
 Operator : SY/MD
 Sample : M2031-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG539

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	9.886	2747	2751	2753	rBV2	358	246	0.01%	0.002%
78	10.040	2796	2799	2805	rBV	382	389	0.02%	0.003%
79	10.130	2822	2827	2828	rBV3	2560	2178	0.13%	0.016%
80	10.223	2843	2856	2878	rBV	621912	962918	56.27%	7.209%
81	10.387	2898	2907	2920	rVB6	3401	5647	0.33%	0.042%
82	10.455	2924	2928	2933	rBV2	802	817	0.05%	0.006%
83	10.750	3016	3020	3021	rBV	514	362	0.02%	0.003%
84	10.805	3035	3037	3042	rBV2	522	404	0.02%	0.003%
85	10.850	3049	3051	3053	rBV2	894	454	0.03%	0.003%
86	10.918	3068	3072	3080	rBV5	4188	4990	0.29%	0.037%
87	11.043	3107	3111	3114	rVB3	804	659	0.04%	0.005%
88	11.062	3114	3117	3123	rBV2	526	589	0.03%	0.004%
89	11.255	3165	3177	3201	rBV	751046	1179498	68.93%	8.831%
90	11.631	3281	3294	3312	rBV	866399	1362277	79.61%	10.199%
91	12.056	3423	3426	3429	rBV3	531	394	0.02%	0.003%
92	12.287	3495	3498	3504	rBV3	547	665	0.04%	0.005%
93	13.078	3743	3744	3747	rBV2	522	313	0.02%	0.002%
94	13.226	3786	3790	3794	rBV4	1098	1054	0.06%	0.008%
95	13.355	3827	3830	3836	rBV3	570	489	0.03%	0.004%
96	13.483	3868	3870	3871	rBV	672	259	0.02%	0.002%
97	14.223	4097	4100	4104	rBV3	645	491	0.03%	0.004%
98	14.381	4147	4149	4152	rBV	754	460	0.03%	0.003%
99	14.496	4181	4185	4189	rBV3	750	850	0.05%	0.006%
100	14.593	4213	4215	4219	rBV	659	432	0.03%	0.003%


Sum of corrected areas: 13356988

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021017.D
Acq On : 14 Apr 2021 19:44
Operator : SY/MD
Sample : M2031-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG539

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

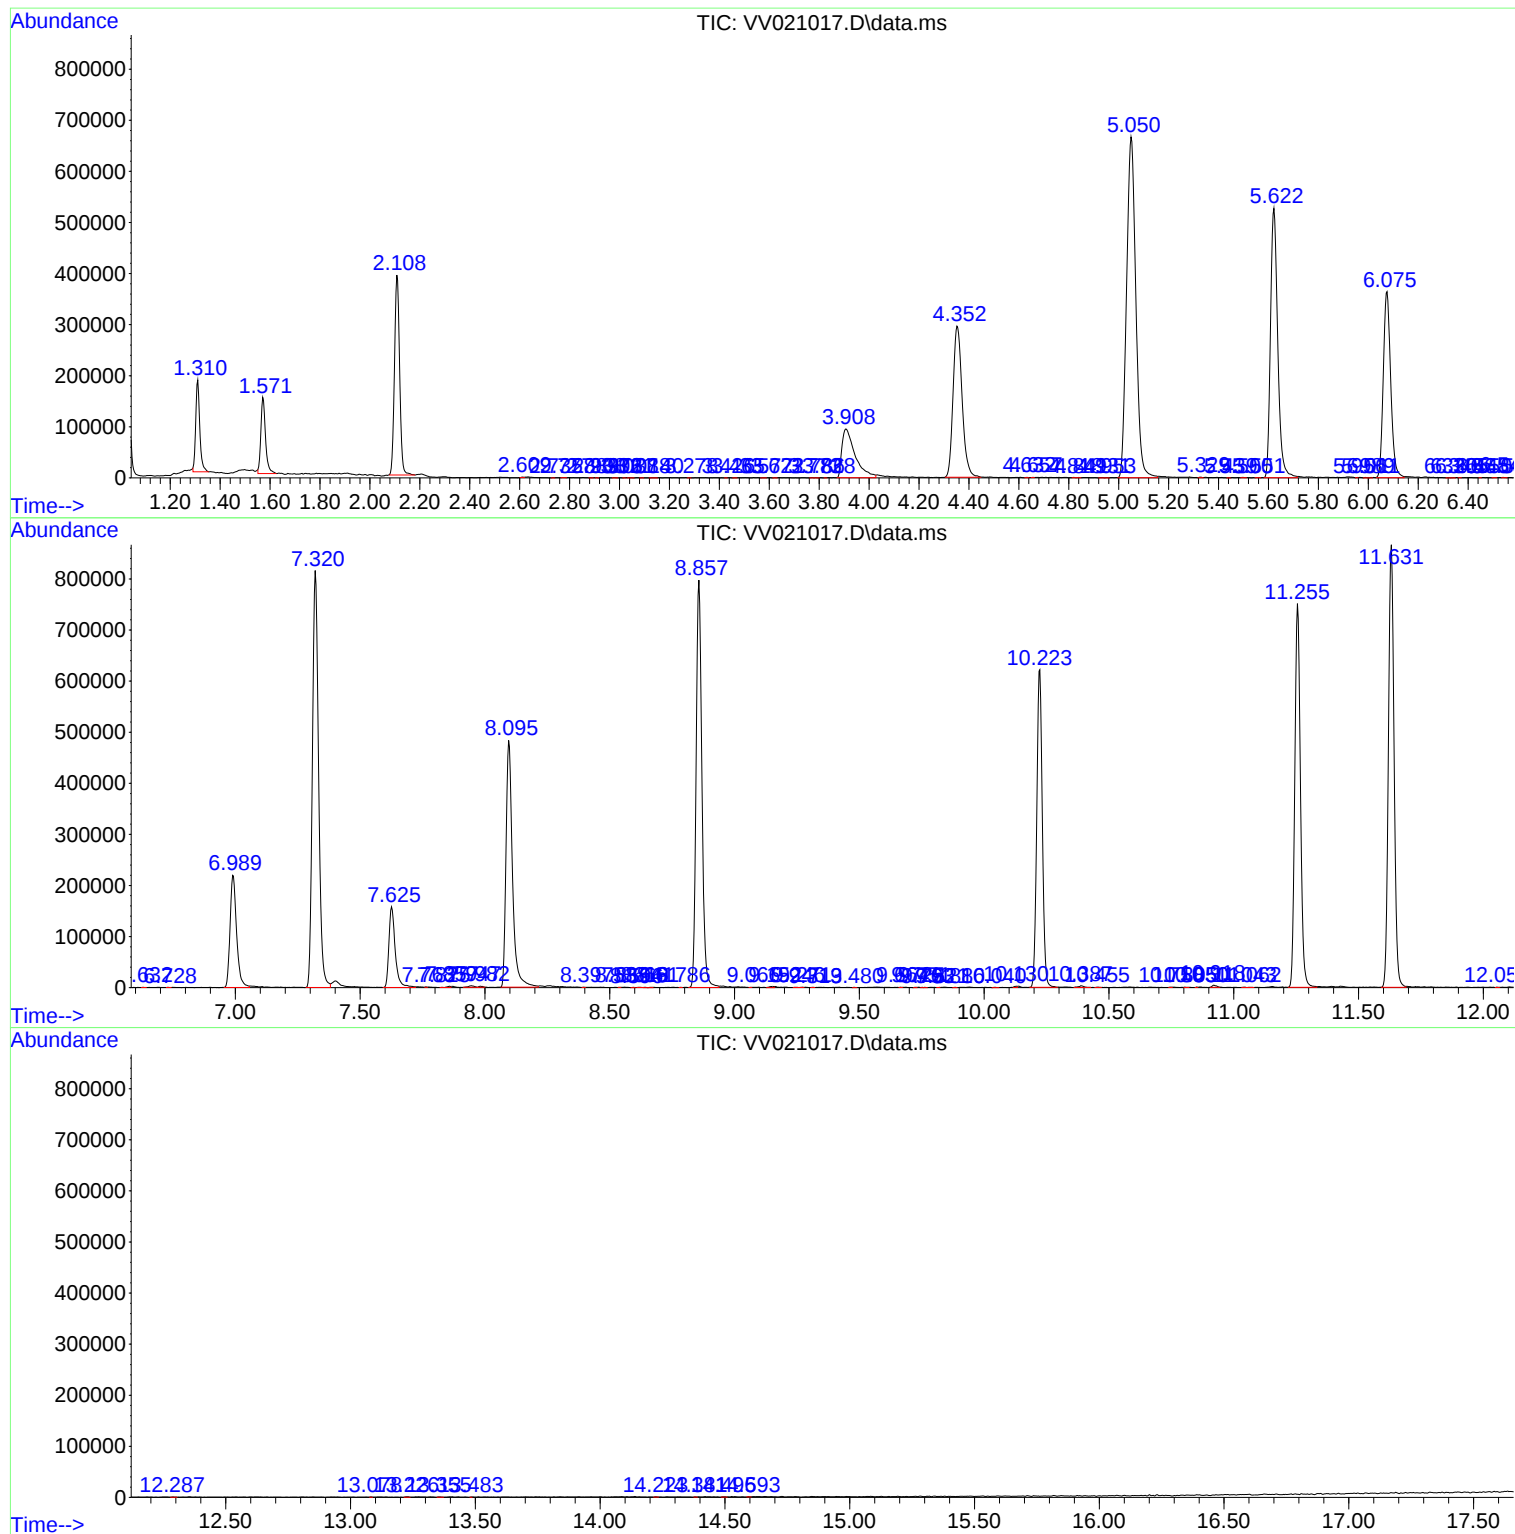

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021017.D
Acq On : 14 Apr 2021 19:44
Operator : SY/MD
Sample : M2031-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG539

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
Data File : VV021017.D
Acq On : 14 Apr 2021 19:44
Operator : SY/MD
Sample : M2031-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG539

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
