

m/z	Abundance
44.10	266.0

Instrument :
MSVOA_V
ClientSampleId :
BFB822

m/z	Abundance
36.10	319.0
37.00	2165.0
38.10	1497.0
39.10	924.0
40.30	111.0
44.00	500.0
45.00	594.0
47.20	480.0
48.30	278.0
49.10	1841.0
50.10	9740.0
51.00	2800.0
52.20	109.0
54.80	172.0
56.00	826.0
57.00	1007.0
60.00	564.0
61.00	2297.0
62.10	3332.0
63.10	1899.0
64.10	534.0
65.10	447.0
67.20	107.0
68.10	6052.0
69.10	5733.0
70.00	446.0
72.10	298.0
73.00	2714.0
74.10	9489.0
75.10	29224.0
76.00	2667.0
77.10	440.0
78.20	252.0
79.00	2065.0
80.10	527.0
81.00	2117.0
82.00	368.0
86.90	2546.0
87.90	2140.0
91.00	312.0
92.00	1937.0
93.00	2447.0
94.10	7810.0
95.10	57288.0
96.10	4021.0
97.10	149.0
103.90	188.0
105.90	268.0
115.80	205.0
117.00	696.0
118.10	351.0
118.90	636.0
127.90	247.0
129.10	225.0
129.90	279.0
135.00	142.0
136.70	172.0
141.00	935.0
142.90	961.0
145.00	292.0
145.70	129.0
147.90	346.0
154.10	160.0
154.90	147.0
156.70	103.0
161.10	136.0
170.70	136.0
171.90	1076.0
173.00	936.0
174.00	54904.0
175.00	4042.0
176.00	54744.0
177.00	3180.0
178.00	260.0

Instrument :
MSVOA_V
ClientSampleId :
BFB822

m/z	Abundance
36.00	487.0
37.00	1981.0
38.10	1710.0
39.10	1061.0
40.30	130.0
44.10	465.0
45.00	466.0
47.00	620.0
48.20	294.0
49.10	1932.0
50.10	10259.0
51.10	2866.0
52.20	111.0
52.80	144.0
54.90	162.0
56.00	855.0
57.00	1031.0
60.10	570.0
61.00	2200.0
62.10	3541.0
63.10	1979.0
64.10	532.0
65.10	557.0
67.20	111.0
68.00	5857.0
69.10	5889.0
70.00	483.0
72.00	280.0
73.10	2798.0
74.10	9784.0
75.10	30272.0
76.00	2523.0
77.10	387.0
78.10	294.0
79.00	2007.0
80.10	429.0
81.00	2273.0
82.00	464.0
86.90	2459.0
87.90	2146.0
90.80	347.0
92.00	2093.0
93.00	2493.0
94.10	7275.0
95.10	59600.0
96.10	4477.0
97.10	150.0
103.80	257.0
105.80	241.0
115.90	234.0
117.00	620.0
118.10	342.0
118.90	475.0
127.90	331.0
129.10	207.0
129.90	335.0
136.80	170.0
140.90	948.0
141.80	126.0
142.90	1092.0
144.90	331.0
148.00	322.0
154.90	216.0
156.70	108.0
161.10	127.0
170.30	105.0
170.80	118.0
171.90	939.0
173.00	919.0
174.00	56120.0
175.00	3993.0
176.00	55360.0
177.00	3223.0
178.00	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB822

m/z	Abundance
36.00	547.0
37.00	1588.0
38.10	1821.0
39.10	942.0
44.00	417.0
45.00	419.0
47.00	586.0
47.90	300.0
48.20	241.0
49.10	1820.0
50.10	9404.0
51.10	2670.0
52.20	116.0
52.80	157.0
55.00	201.0
56.00	827.0
57.10	1023.0
58.20	104.0
60.10	549.0
61.00	2132.0
62.10	3183.0
63.10	2021.0
64.10	380.0
65.10	625.0
68.00	4985.0
69.10	5426.0
69.90	430.0
71.90	273.0
73.10	2589.0
74.10	9579.0
75.10	28488.0
76.00	2437.0
77.00	256.0
78.10	330.0
79.00	1963.0
79.90	321.0
81.00	2302.0
82.10	478.0
85.80	108.0
87.00	2234.0
87.90	1956.0
90.80	318.0
92.00	1910.0
93.10	2340.0
94.00	6232.0
95.10	56312.0
96.10	3981.0
97.20	146.0
103.80	275.0
105.00	107.0
105.70	193.0
106.20	104.0
115.90	234.0
116.90	429.0
118.10	277.0
118.90	323.0
127.90	299.0
129.10	165.0
130.00	318.0
135.20	113.0
136.80	176.0
140.90	903.0
141.80	174.0
142.90	1063.0
145.00	407.0
148.00	209.0
152.60	105.0
154.90	225.0
170.30	110.0
170.80	140.0
171.90	745.0
173.00	820.0
174.00	51696.0
175.00	3471.0
176.00	50568.0
176.90	3172.0


Instrument :
MSVOA_V
ClientSampleId :
BFB822

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041421\
 Data File : VV021003.D
 Acq On : 14 Apr 2021 13:24
 Operator : SY/MD
 Sample : BFB82
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB822

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis
 Last Update : Thu Apr 15 01:36:39 2021

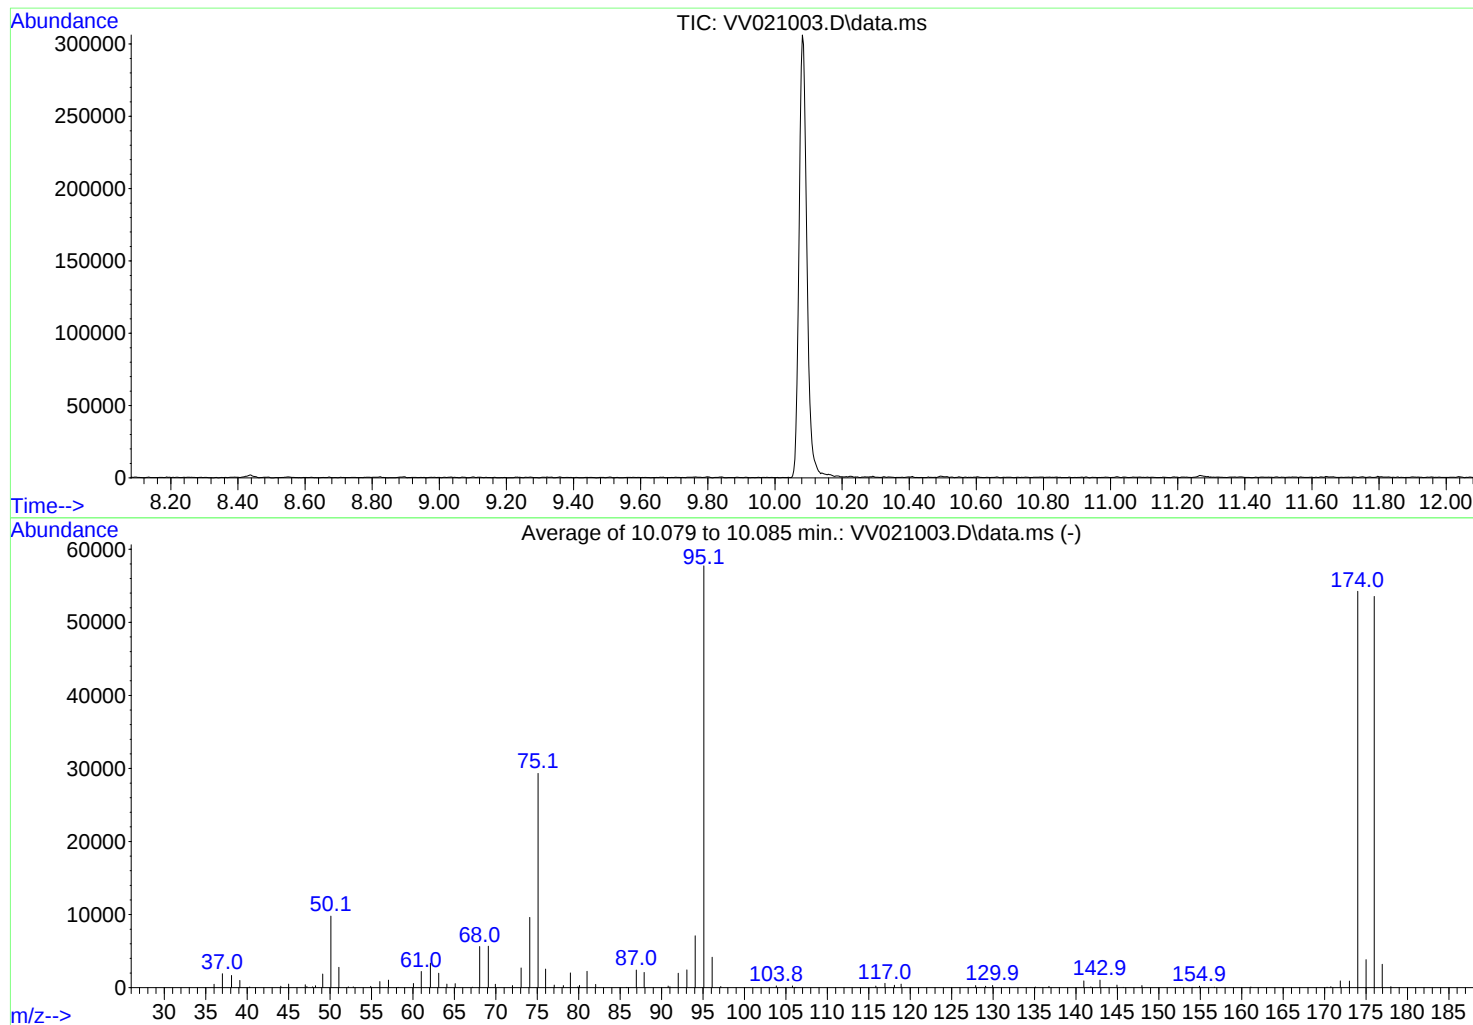

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	9801	PASS
75	95	30	80	50.8	29328	PASS
95	95	100	100	100.0	57733	PASS
96	95	5	9	7.2	4160	PASS
173	174	0.00	2	1.6	892	PASS
174	95	50	120	93.9	54240	PASS
175	174	5	9	7.1	3835	PASS
176	174	95	101	98.7	53557	PASS
177	176	5	9	6.0	3192	PASS