

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041423\
 Data File : VW030568.D
 Acq On : 14 Apr 2023 13:14
 Operator : SY/MD
 Sample : 02275-06DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDZ2DL

Quant Time: Apr 15 01:58:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 15 01:54:33 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	119777	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.796	117	116238	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	55095	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	43451	5.477	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	109.600%	
7) Chloroethane-d5	1.536	69	35141	4.565	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	91.200%	
11) 1,1-Dichloroethene-d2	2.063	63	66585	3.537	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	70.800%	
20) 2-Butanone-d5	3.831	46	81384	39.691	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	79.380%	
24) Chloroform-d	4.262	84	80121	4.173	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	83.400%	
26) 1,2-Dichloroethane-d4	4.957	65	42996	4.746	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.000%	
32) Benzene-d6	4.970	84	138019	4.214	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	84.200%	
36) 1,2-Dichloropropane-d6	5.998	67	45702	4.457	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	89.200%	
41) Toluene-d8	7.252	98	119364	3.968	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	79.400%	
43) trans-1,3-Dichloroprop...	7.564	79	16485	4.270	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	85.400%	
46) 2-Hexanone-d5	8.037	63	65490	42.212	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	84.420%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	32506	4.022	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	80.400%	
66) 1,2-Dichlorobenzene-d4	11.571	152	44395	4.508	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	90.200%	
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.066	101	2326	0.206	ug/L #	81
12) 1,1-Dichloroethene	2.069	96	2261	0.226	ug/L #	1
22) cis-1,2-Dichloroethene	3.831	96	9098	0.860	ug/L #	97
34) Trichloroethene	5.844	95	28776	2.584	ug/L	98
47) Tetrachloroethene	7.915	164	89673	9.125	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030568.D
Acq On : 14 Apr 2023 13:14
Operator : SY/MD
Sample : 02275-06DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ2DL

Quant Time: Apr 15 01:58:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 15 01:54:33 2023
Response via : Initial Calibration




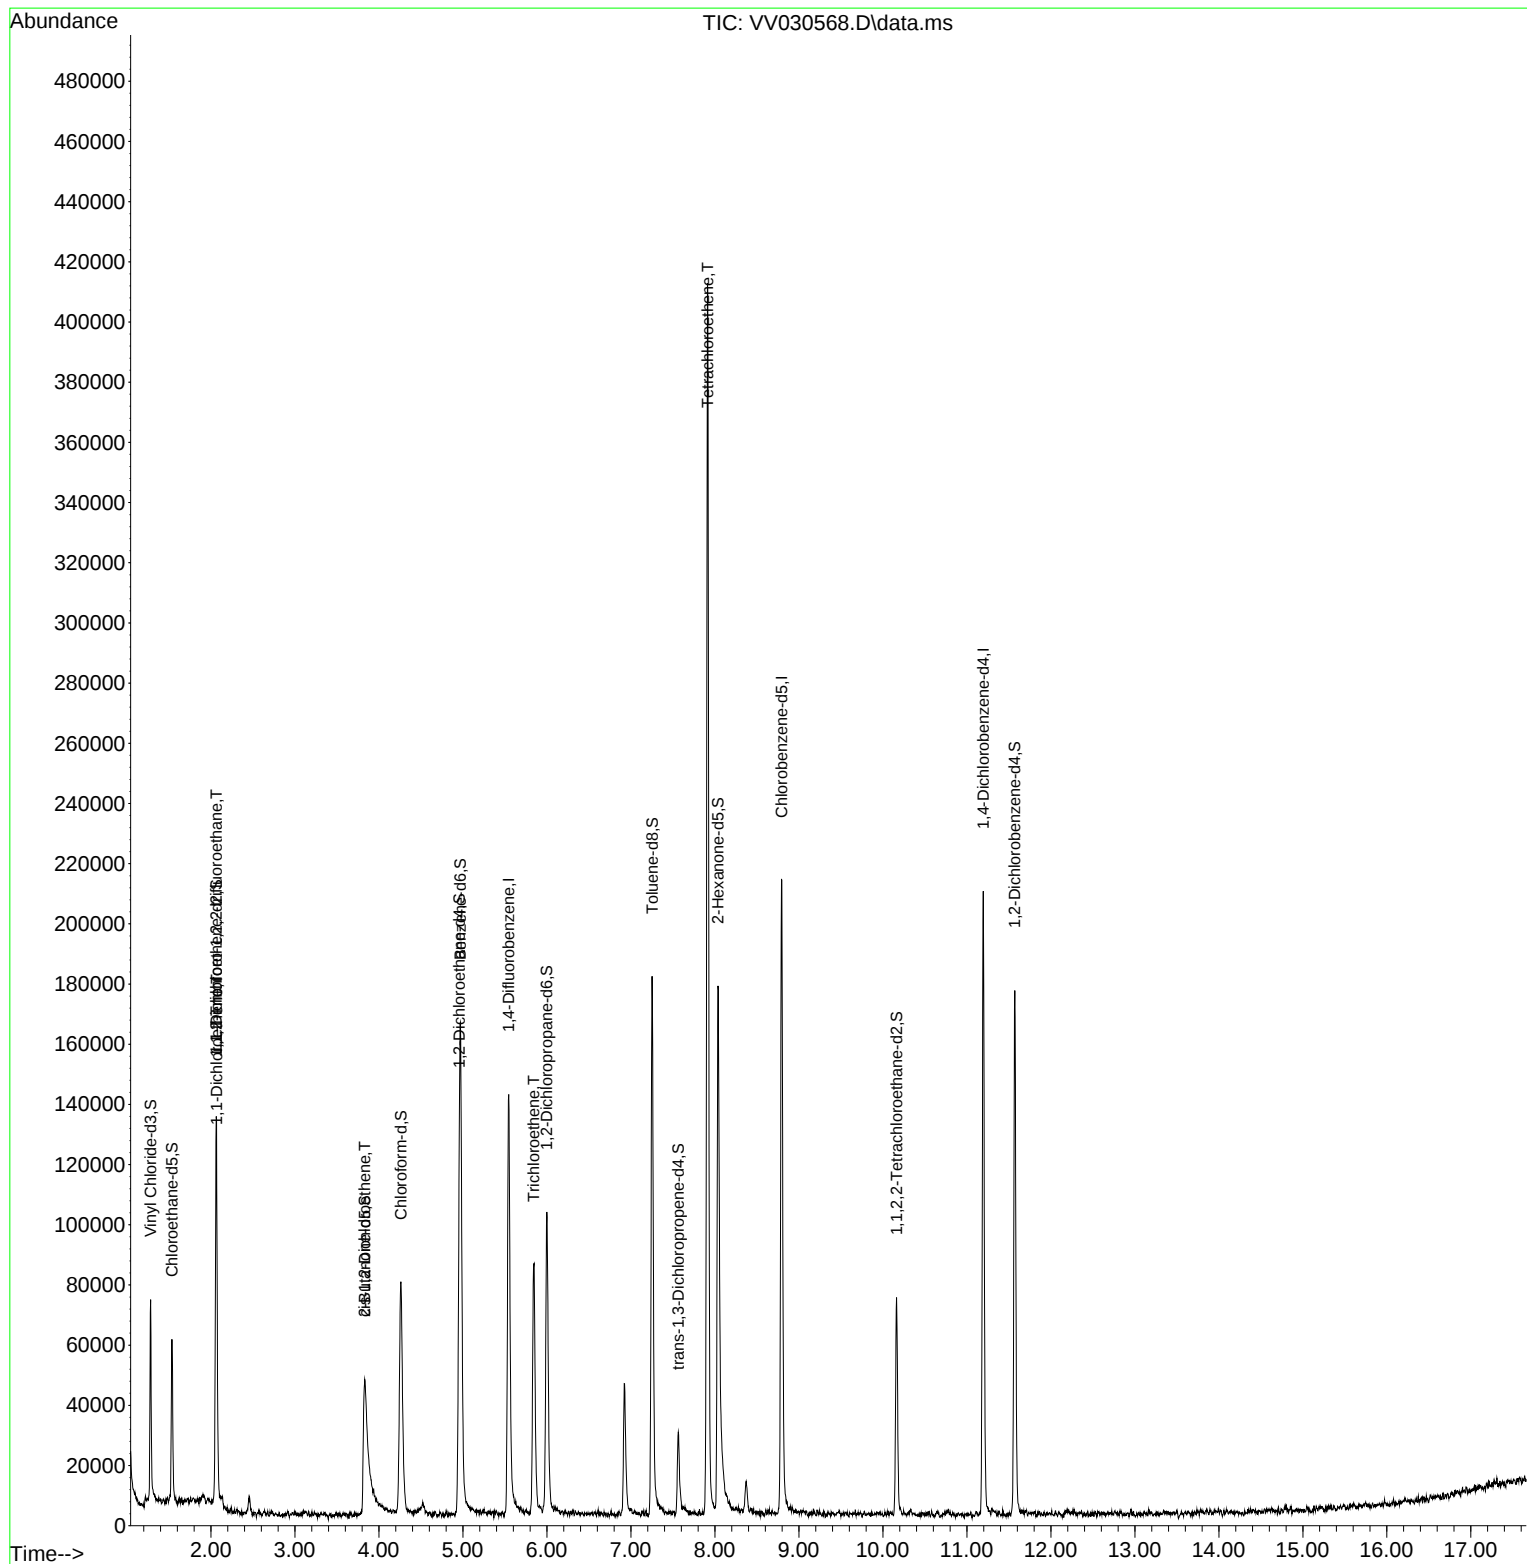


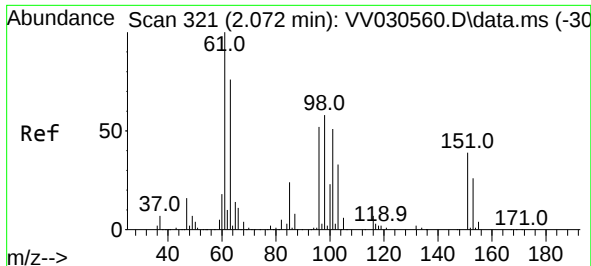

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.206 ug/L
 RT: 2.066 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VV030568.D
 Acq: 14 Apr 2023 13:14




Instrument :
 MSVOA_V
 ClientSampleId :
 BHDZ2DL


Tgt Ion:101 Resp: 2326
 Ion Ratio Lower Upper
 101 100
 85 37.4 38.1 57.1#
 151 59.2 62.7 94.1#

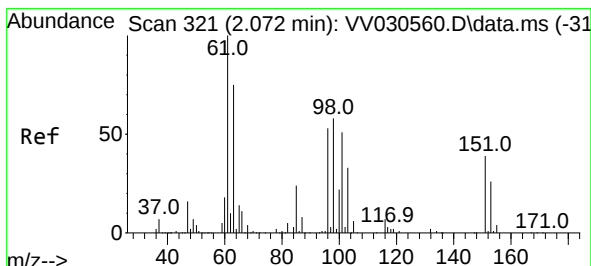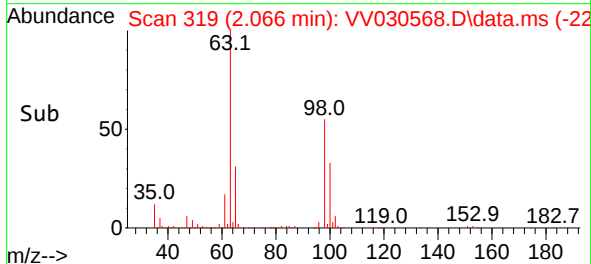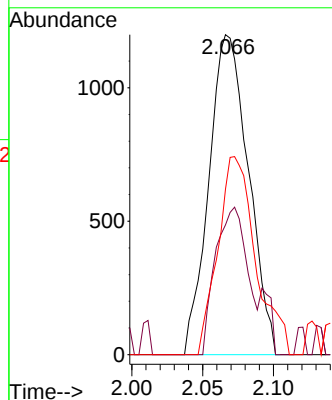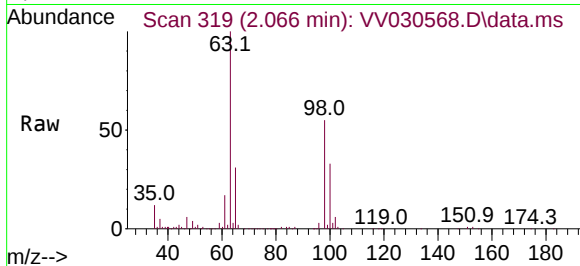

#12
 1,1-Dichloroethene
 Concen: 0.226 ug/L
 RT: 2.069 min Scan# 320
 Delta R.T. -0.003 min
 Lab File: VV030568.D
 Acq: 14 Apr 2023 13:14

Tgt Ion: 96 Resp: 2261
 Ion Ratio Lower Upper
 96 100
 61 495.8 136.3 253.1#
 63 2869.2 92.1 171.1#


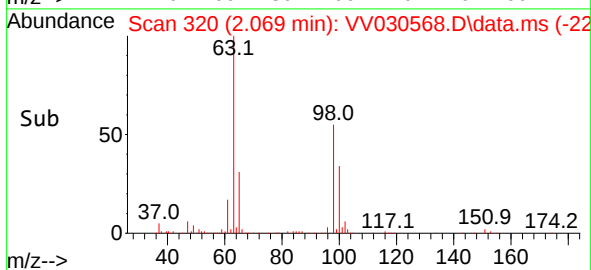
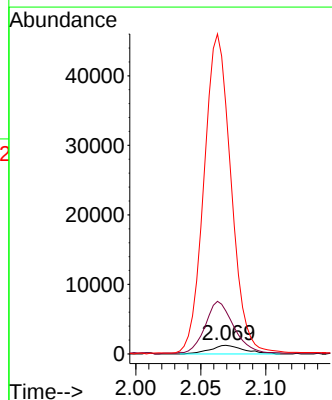
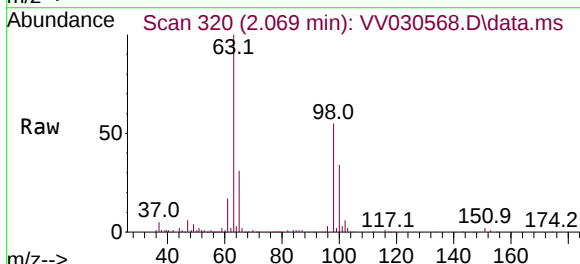


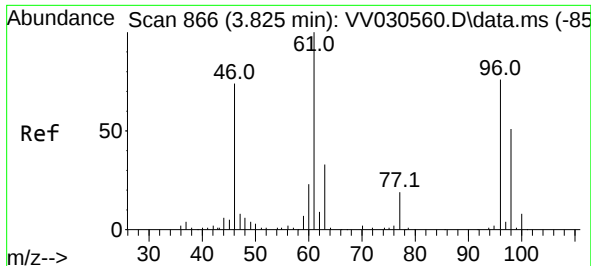

#22
 cis-1,2-Dichloroethene
 Concen: 0.860 ug/L
 RT: 3.831 min Scan# 866
 Delta R.T. 0.007 min
 Lab File: VV030568.D
 Acq: 14 Apr 2023 13:14




Instrument :
 MSVOA_V
 ClientSampleId :
 BHDZ2DL


Tgt Ion: 96 Resp: 9098
 Ion Ratio Lower Upper
 96 100
 61 135.3 92.0 170.8
 68 3.0 0.0 0.0#

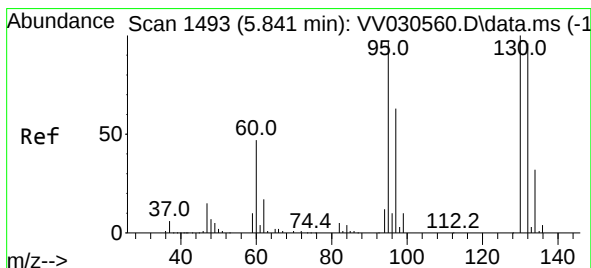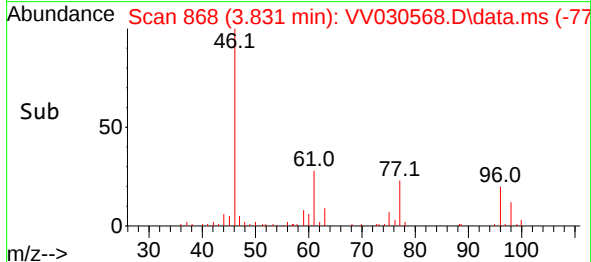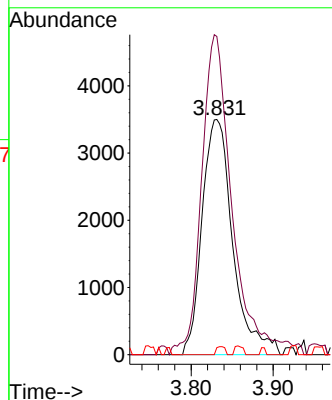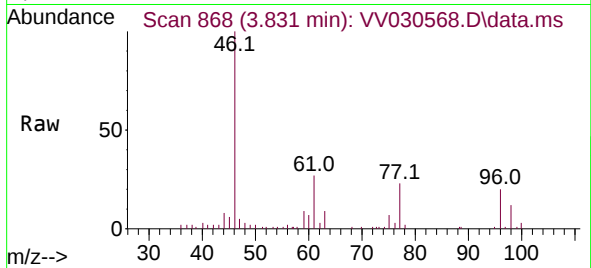

#34
 Trichloroethene
 Concen: 2.584 ug/L
 RT: 5.844 min Scan# 1494
 Delta R.T. 0.003 min
 Lab File: VV030568.D
 Acq: 14 Apr 2023 13:14


Tgt Ion: 95 Resp: 28776
 Ion Ratio Lower Upper
 95 100
 97 63.8 44.2 82.2
 132 96.2 69.5 129.1
 130 105.9 72.2 134.0

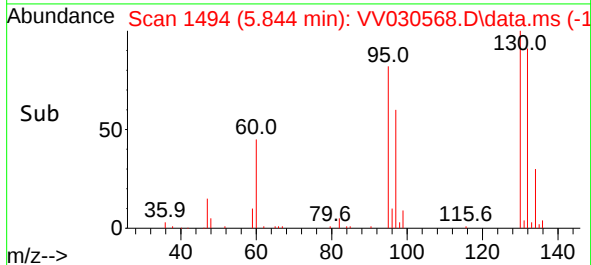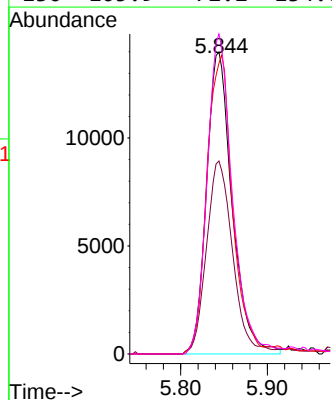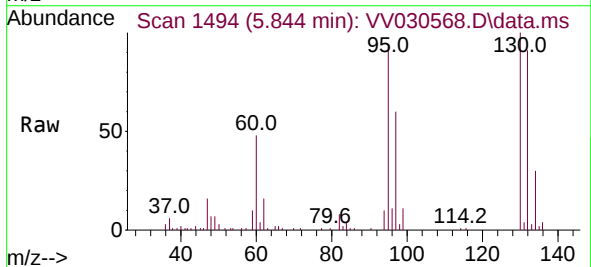

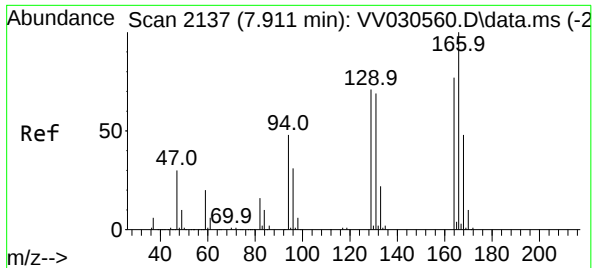

#47
 Tetrachloroethene
 Concen: 9.125 ug/L
 RT: 7.915 min Scan# 21
 Delta R.T. 0.003 min
 Lab File: VV030568.D
 Acq: 14 Apr 2023 13:14

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDZ2DL

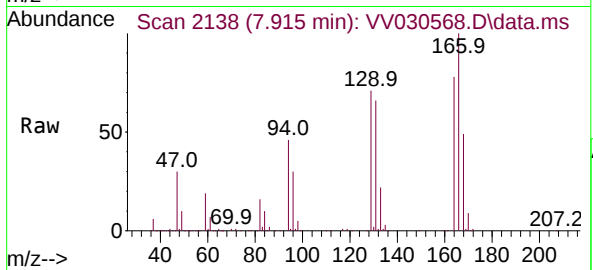

Tgt Ion:	164	Resp:	89673
Ion	Ratio	Lower	Upper
164	100		
129	90.8	60.8	112.8
131	85.2	61.7	114.7
166	128.2	85.6	159.0

