

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
 Data File : VV030568.D
 Acq On : 14 Apr 2023 13:14
 Operator : SY/MD
 Sample : 02275-06DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDZ2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030568.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	94	rVB	66517	73838	10.50%	1.656%
2	1.536	148	154	165	rVB	53345	65499	9.32%	1.469%
3	2.063	307	318	330	rBV	127601	192417	27.37%	4.315%
4	2.458	435	441	451	rVB	5969	9826	1.40%	0.220%
5	3.831	857	868	898	rBV2	44045	168687	23.99%	3.783%
6	4.262	985	1002	1022	rBV2	76764	199464	28.37%	4.474%
7	4.970	1206	1222	1243	rBV2	162808	413626	58.83%	9.277%
8	5.545	1389	1401	1426	rBV	138438	292137	41.55%	6.552%
9	5.847	1478	1495	1512	rBV2	83618	178363	25.37%	4.000%
10	5.998	1530	1542	1562	rVB	98355	199912	28.43%	4.484%
11	6.921	1815	1829	1845	rBV	43900	86438	12.29%	1.939%
12	7.252	1918	1932	1952	rBV	179414	331700	47.18%	7.439%
13	7.564	2018	2029	2043	rBV2	27612	53597	7.62%	1.202%
14	7.912	2123	2137	2162	rBV	409084	703084	100.00%	15.769%
15	8.037	2166	2176	2205	rBV	173316	366850	52.18%	8.228%
16	8.371	2268	2280	2293	rBV4	10470	21338	3.03%	0.479%
17	8.793	2397	2411	2429	rBV	210553	361529	51.42%	8.108%
18	10.162	2826	2837	2849	rBV	72525	120940	17.20%	2.712%
19	11.194	3147	3158	3177	rBV	206974	329225	46.83%	7.384%
20	11.571	3260	3275	3294	rBV	174678	290281	41.29%	6.510%




Sum of corrected areas: 4458751

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030568.D
Acq On : 14 Apr 2023 13:14
Operator : SY/MD
Sample : 02275-06DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

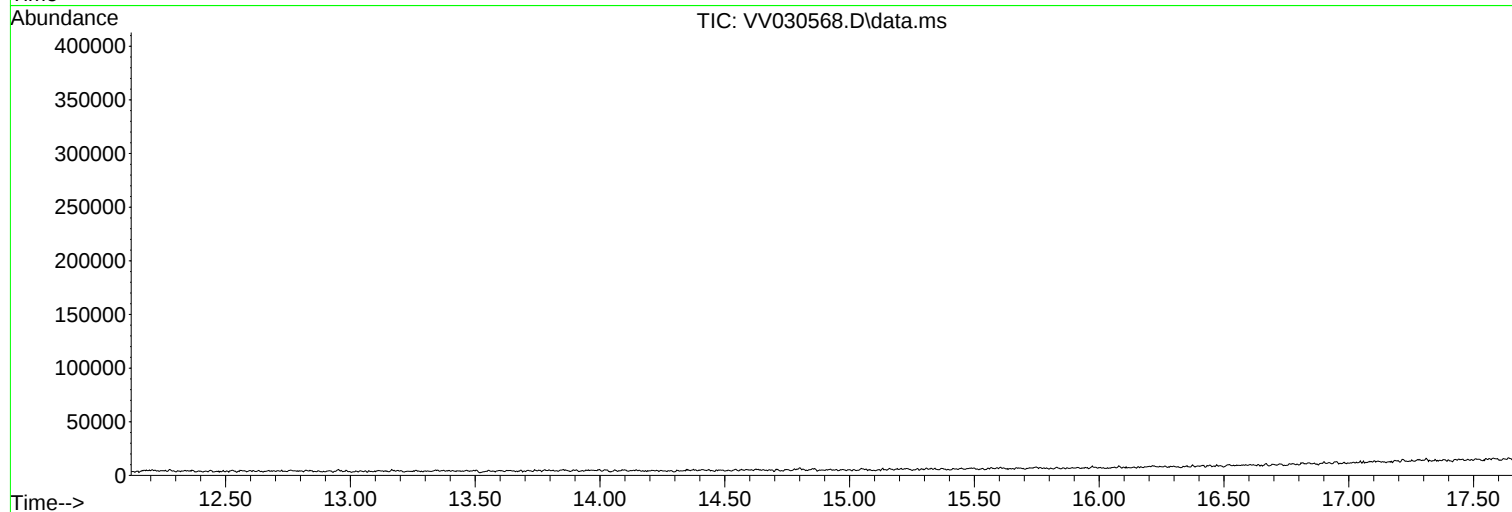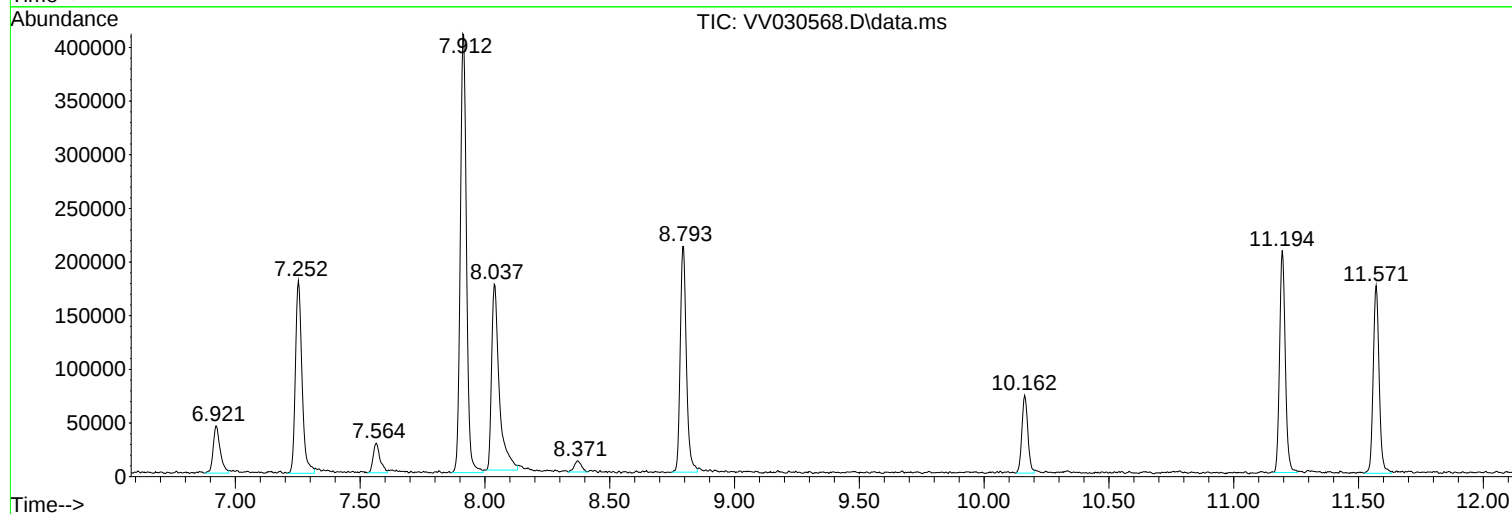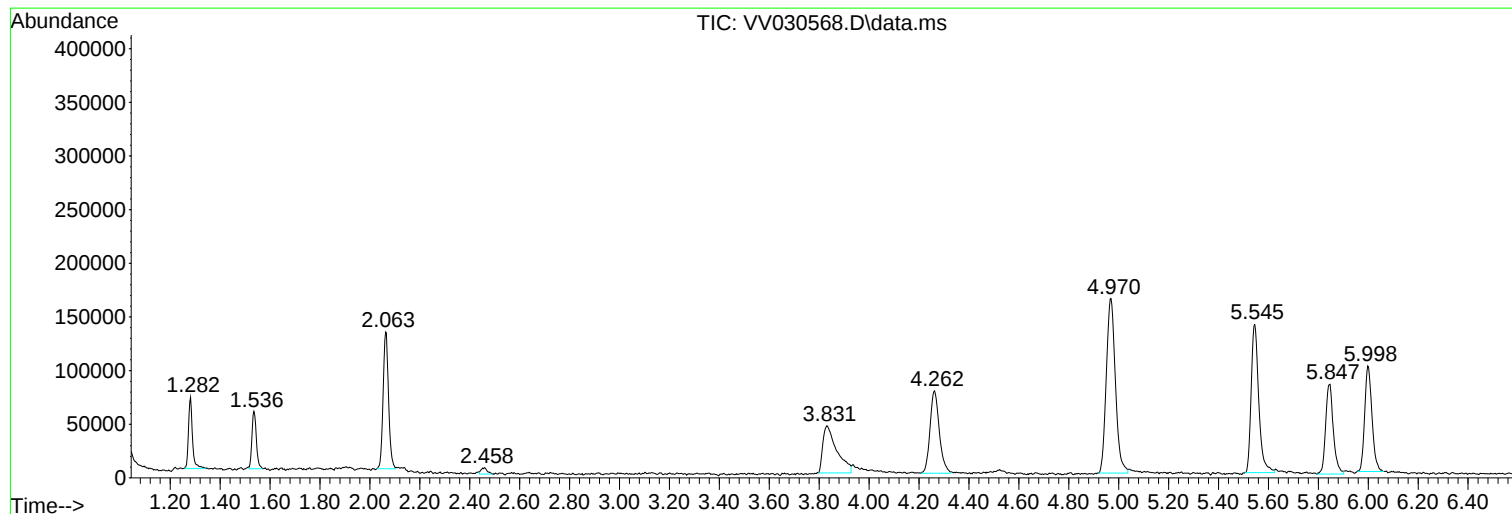

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030568.D
Acq On : 14 Apr 2023 13:14
Operator : SY/MD
Sample : 02275-06DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030568.D
Acq On : 14 Apr 2023 13:14
Operator : SY/MD
Sample : 02275-06DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------