

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
 Data File : VV030570.D
 Acq On : 14 Apr 2023 14:02
 Operator : SY/MD
 Sample : 02275-14DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDZ9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	61	rBV6	3696	4668	1.09%	0.113%
2	1.281	61	75	87	rVV	64194	77063	17.92%	1.861%
3	1.535	148	154	167	rVB	54524	63318	14.72%	1.529%
4	2.063	308	318	330	rBV2	117098	171960	39.98%	4.152%
5	2.458	431	441	446	rBV8	4297	7355	1.71%	0.178%
6	3.831	853	868	898	rBV3	67430	229955	53.47%	5.552%
7	4.259	982	1001	1023	rBV	73904	195077	45.36%	4.710%
8	4.969	1206	1222	1250	rBV3	160305	409802	95.29%	9.894%
9	5.545	1385	1401	1421	rBV	130760	280310	65.18%	6.768%
10	5.841	1478	1493	1510	rBV	212120	430071	100.00%	10.383%
11	5.998	1530	1542	1559	rBV2	94742	194154	45.14%	4.688%
12	6.921	1821	1829	1843	rBV	40131	76330	17.75%	1.843%
13	7.252	1921	1932	1951	rBV	166485	308011	71.62%	7.436%
14	7.564	2020	2029	2050	rBV2	25625	53205	12.37%	1.285%
15	7.915	2125	2138	2151	rBV	120003	206072	47.92%	4.975%
16	8.040	2166	2177	2205	rBV	166002	369953	86.02%	8.932%
17	8.374	2272	2281	2291	rVB5	7008	13249	3.08%	0.320%
18	8.792	2397	2411	2433	rBV	202040	351489	81.73%	8.486%
19	10.162	2826	2837	2851	rBV	71909	116380	27.06%	2.810%
20	11.194	3147	3158	3176	rBV	192672	310953	72.30%	7.508%
21	11.570	3263	3275	3290	rBV	170589	272523	63.37%	6.580%




Sum of corrected areas: 4141898

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030570.D
Acq On : 14 Apr 2023 14:02
Operator : SY/MD
Sample : 02275-14DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

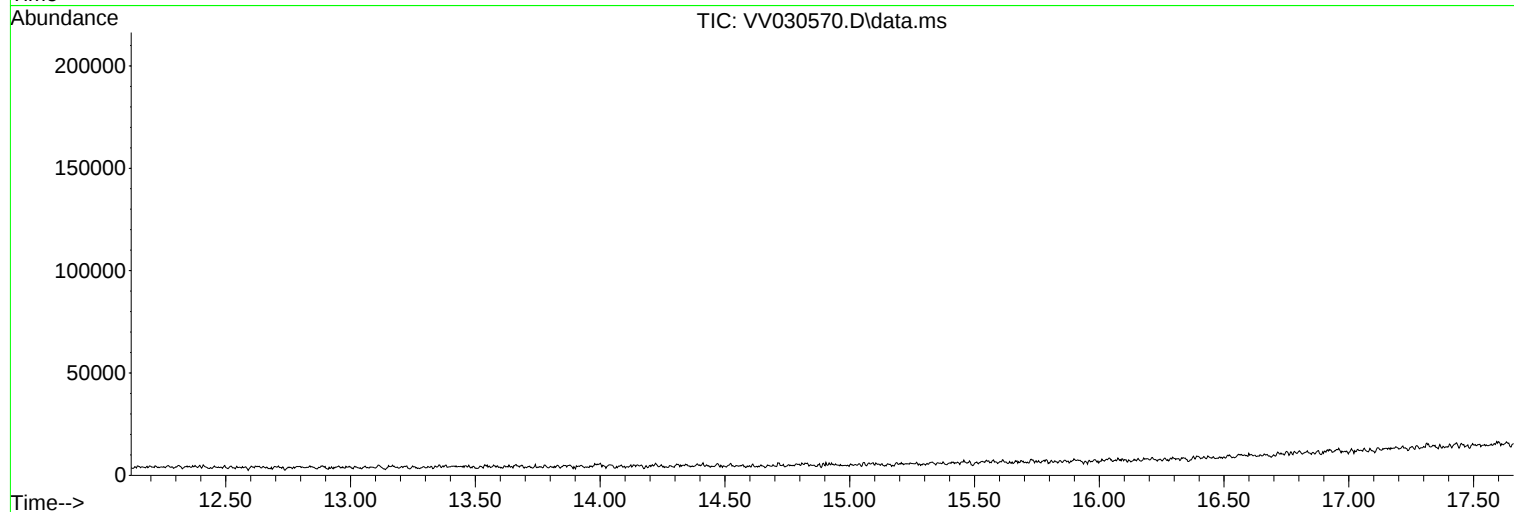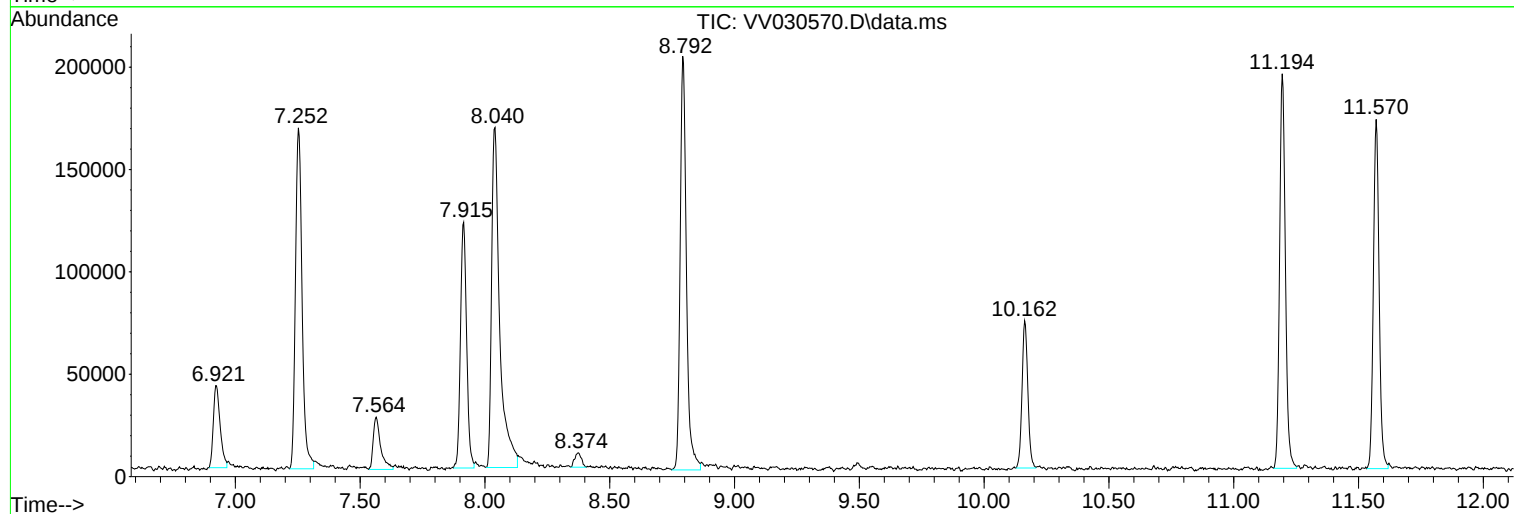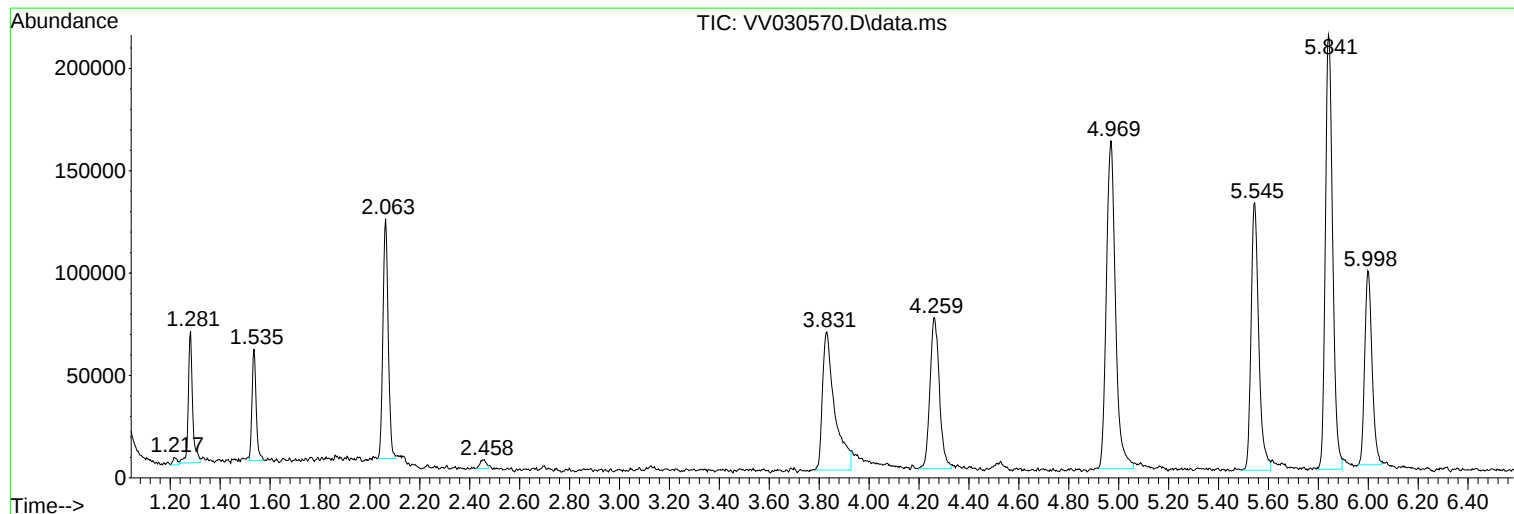

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030570.D
Acq On : 14 Apr 2023 14:02
Operator : SY/MD
Sample : 02275-14DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030570.D
Acq On : 14 Apr 2023 14:02
Operator : SY/MD
Sample : 02275-14DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------