

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
 Data File : VV030571.D
 Acq On : 14 Apr 2023 14:24
 Operator : SY/MD
 Sample : 02275-15DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE00DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030571.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rBV	58285	65560	12.20%	1.611%
2	1.536	146	154	164	rBV	55777	65409	12.17%	1.607%
3	2.063	307	318	331	rBV	119013	176652	32.88%	4.340%
4	2.455	432	440	449	rVB6	4307	7339	1.37%	0.180%
5	3.834	857	869	886	rBV2	31003	108685	20.23%	2.670%
6	4.265	985	1003	1028	rBV3	76517	196066	36.49%	4.817%
7	4.969	1205	1222	1244	rBV3	160115	411359	76.56%	10.106%
8	5.545	1385	1401	1421	rBV	132602	281020	52.30%	6.904%
9	5.844	1482	1494	1511	rBV2	82478	173745	32.34%	4.268%
10	6.002	1531	1543	1560	rBV2	95116	198032	36.86%	4.865%
11	6.924	1820	1830	1845	rBV2	41246	77669	14.46%	1.908%
12	7.252	1921	1932	1949	rBV	167988	305025	56.77%	7.494%
13	7.564	2019	2029	2045	rBV	26175	48239	8.98%	1.185%
14	7.915	2125	2138	2159	rBV	310623	537275	100.00%	13.199%
15	8.040	2167	2177	2213	rBV	173258	371682	69.18%	9.131%
16	8.378	2270	2282	2288	rBV10	5884	10810	2.01%	0.266%
17	8.796	2400	2412	2427	rBV	196596	333226	62.02%	8.186%
18	10.162	2826	2837	2851	rBV	71299	115515	21.50%	2.838%
19	11.194	3146	3158	3177	rBV	195997	311044	57.89%	7.641%
20	11.571	3262	3275	3292	rBV	168466	276148	51.40%	6.784%




Sum of corrected areas: 4070500

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030571.D
Acq On : 14 Apr 2023 14:24
Operator : SY/MD
Sample : 02275-15DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

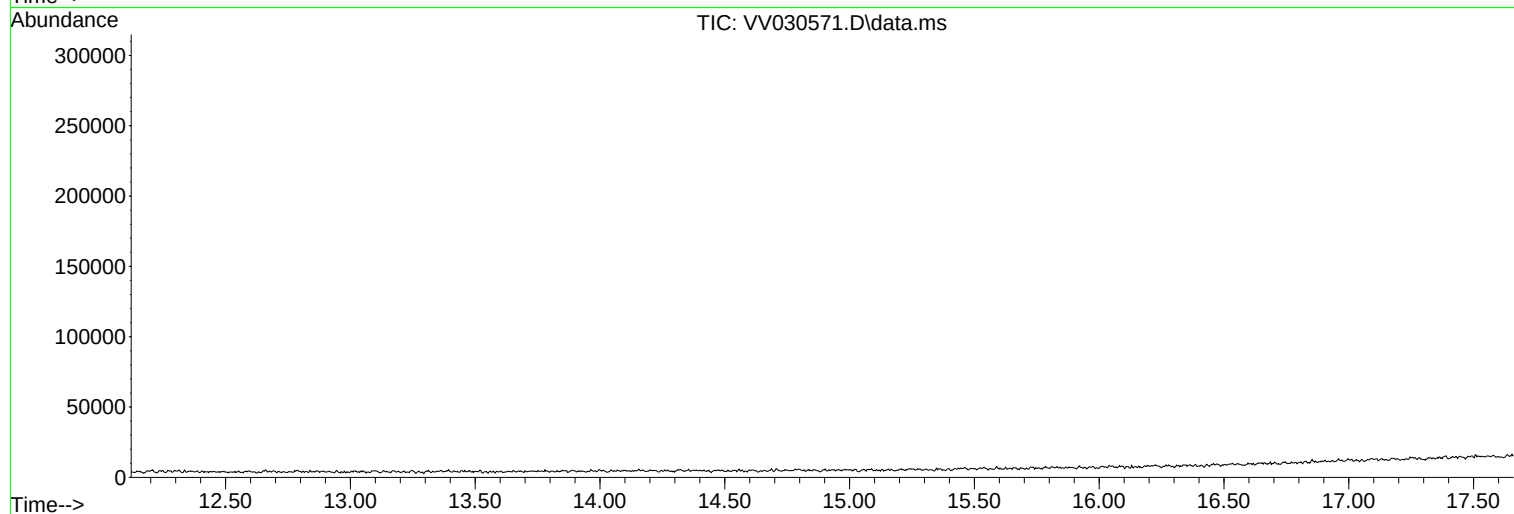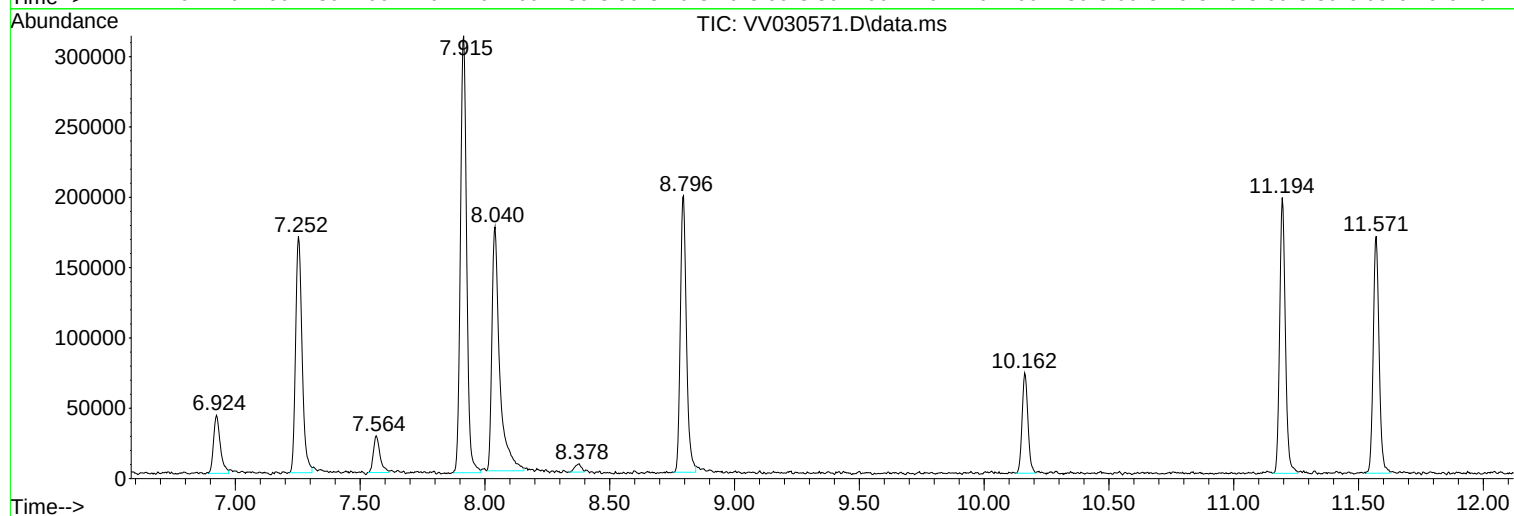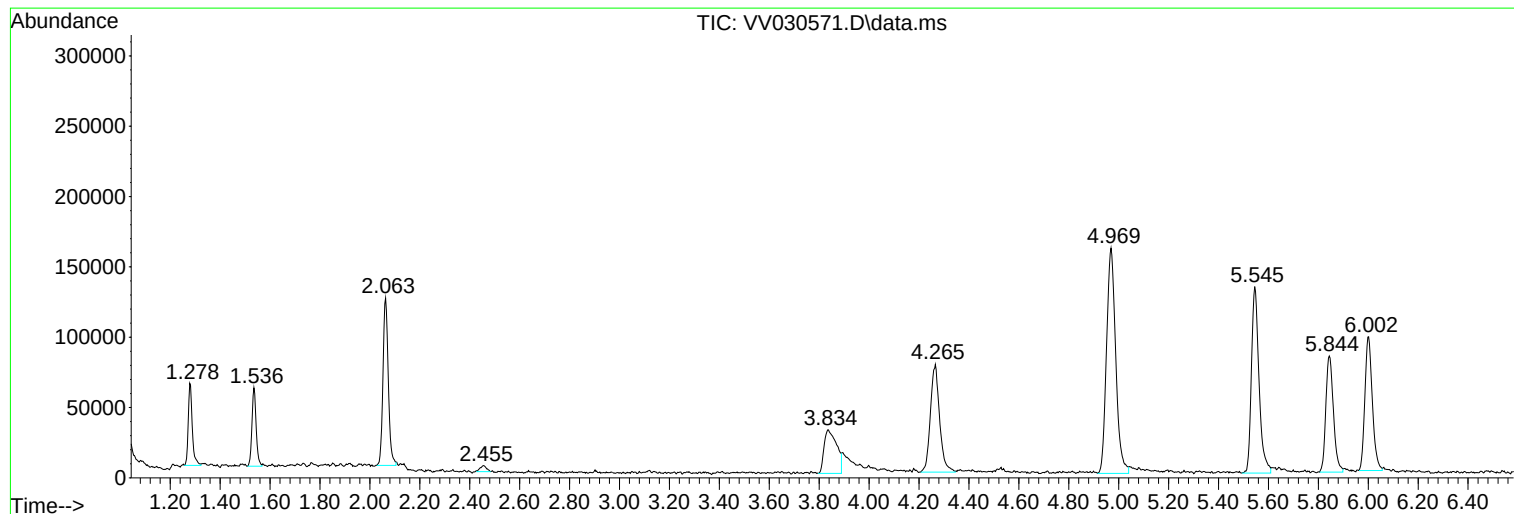

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030571.D
Acq On : 14 Apr 2023 14:24
Operator : SY/MD
Sample : 02275-15DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030571.D
Acq On : 14 Apr 2023 14:24
Operator : SY/MD
Sample : 02275-15DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------