

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
 Data File : VV030573.D
 Acq On : 14 Apr 2023 15:12
 Operator : SY/MD
 Sample : 02275-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDZ4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030573.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	59	rBV5	3573	4190	1.14%	0.141%
2	1.282	68	75	83	rBV	43603	47806	13.02%	1.609%
3	1.536	146	154	165	rBV	38987	48292	13.15%	1.625%
4	2.063	308	318	329	rBV	86278	125279	34.12%	4.216%
5	2.243	368	374	379	rBV4	3125	4151	1.13%	0.140%
6	2.455	430	440	444	rBV4	3609	5545	1.51%	0.187%
7	3.815	853	863	888	rBV2	44395	144907	39.47%	4.876%
8	4.262	986	1002	1021	rBV2	56243	149608	40.75%	5.034%
9	4.523	1072	1083	1084	rBV9	4636	5402	1.47%	0.182%
10	4.970	1205	1222	1242	rBV3	119110	311406	84.82%	10.479%
11	5.545	1390	1401	1423	rBV2	104946	224668	61.19%	7.560%
12	5.850	1486	1496	1500	rBV2	4524	7278	1.98%	0.245%
13	6.002	1526	1543	1562	rBV2	75323	163298	44.48%	5.495%
14	6.924	1817	1830	1845	rBV	33185	68146	18.56%	2.293%
15	7.252	1921	1932	1946	rBV	124042	223586	60.90%	7.524%
16	7.330	1948	1956	1967	rVB	16560	32946	8.97%	1.109%
17	7.564	2018	2029	2041	rBV2	22211	41776	11.38%	1.406%
18	7.892	2116	2131	2136	rBV	15823	31573	8.60%	1.062%
19	8.037	2164	2176	2204	rBV	177560	367141	100.00%	12.354%
20	8.796	2396	2412	2430	rBV	162051	281462	76.66%	9.471%
21	9.510	2627	2634	2639	rBV7	3626	4767	1.30%	0.160%
22	9.764	2706	2713	2719	rBV7	3204	3941	1.07%	0.133%
23	10.162	2825	2837	2849	rBV	67145	110748	30.16%	3.727%
24	10.336	2880	2891	2902	rVB2	32728	58031	15.81%	1.953%
25	11.194	3148	3158	3172	rBV	159038	255313	69.54%	8.591%
26	11.571	3264	3275	3289	rBV	137136	215822	58.78%	7.262%
27	12.207	3464	3473	3483	rVB3	9450	14617	3.98%	0.492%
28	12.297	3491	3501	3512	rBV8	12664	20045	5.46%	0.675%




Sum of corrected areas: 2971744

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030573.D
Acq On : 14 Apr 2023 15:12
Operator : SY/MD
Sample : 02275-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

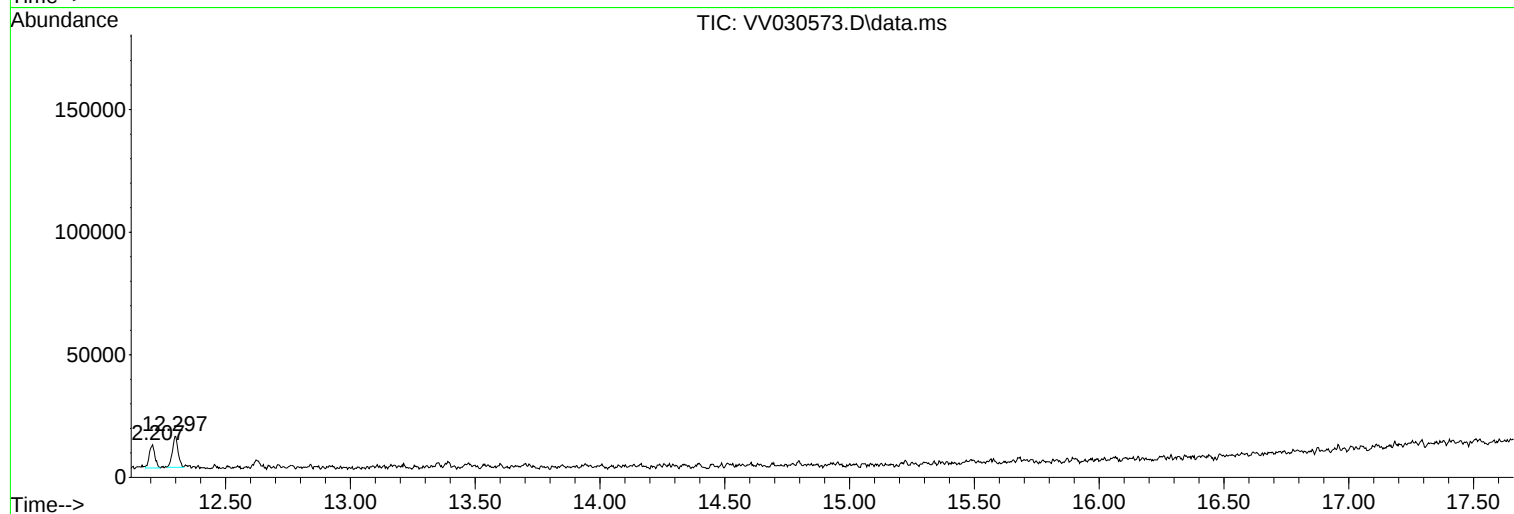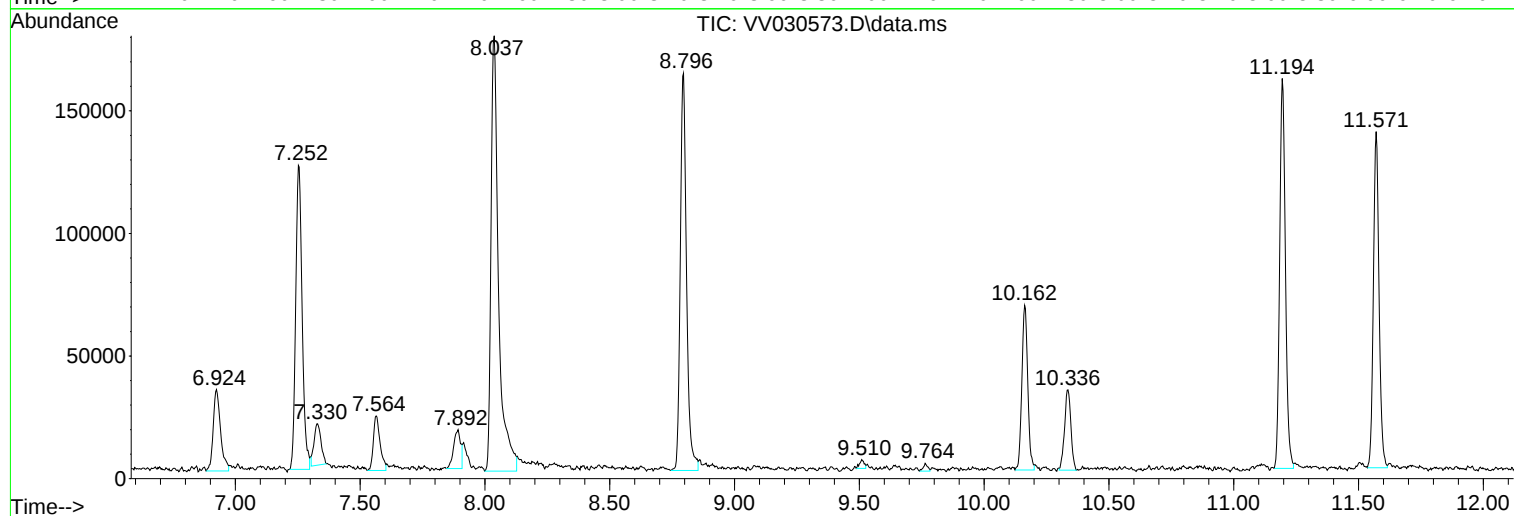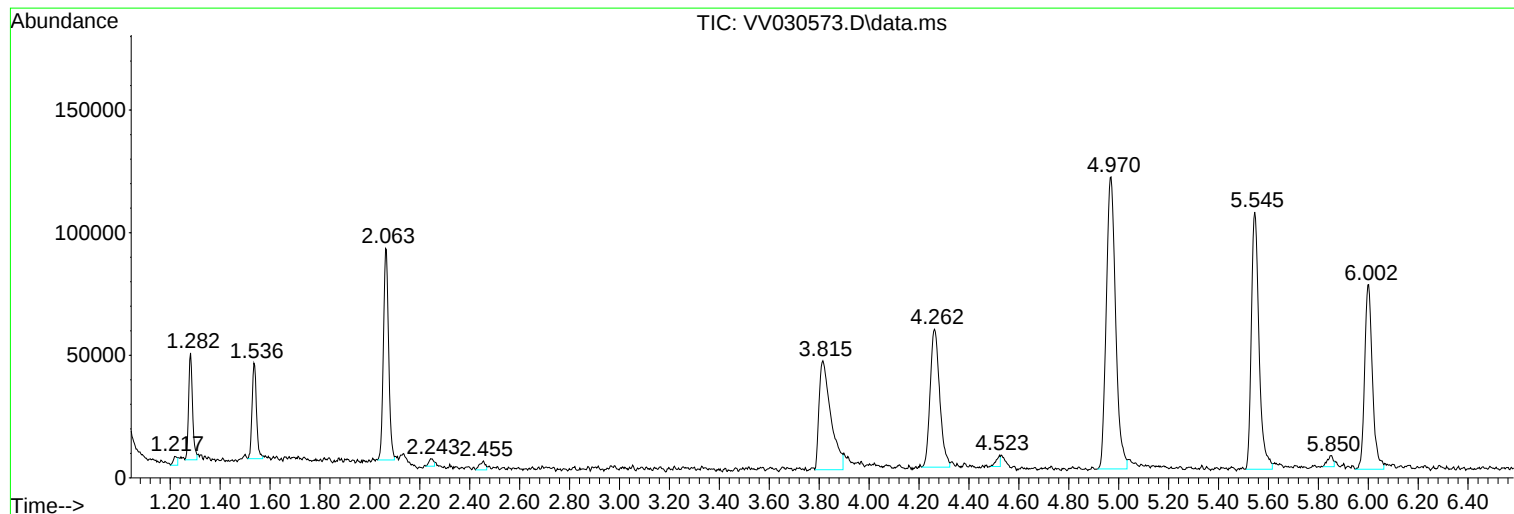

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030573.D
Acq On : 14 Apr 2023 15:12
Operator : SY/MD
Sample : 02275-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030573.D
Acq On : 14 Apr 2023 15:12
Operator : SY/MD
Sample : 02275-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDZ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------