

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
 Data File : VV030575.D
 Acq On : 14 Apr 2023 15:58
 Operator : SY/MD
 Sample : 02275-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030575.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	86	rBV	57280	64621	16.13%	1.878%
2	1.539	146	155	170	rVV	51157	65121	16.26%	1.892%
3	2.063	308	318	330	rBV	112176	165856	41.41%	4.820%
4	3.822	853	865	889	rBV2	41039	149808	37.40%	4.353%
5	4.262	988	1002	1022	rBV2	77640	188052	46.95%	5.465%
6	4.969	1205	1222	1242	rBV2	156679	400569	100.00%	11.640%
7	5.545	1389	1401	1420	rBV	128142	270223	67.46%	7.852%
8	5.998	1528	1542	1563	rBV2	95753	204745	51.11%	5.950%
9	6.924	1820	1830	1842	rBV2	41337	78096	19.50%	2.269%
10	7.252	1919	1932	1946	rBV	166907	297685	74.32%	8.650%
11	7.564	2015	2029	2040	rBV2	25433	48000	11.98%	1.395%
12	7.886	2118	2129	2140	rBV	9920	18631	4.65%	0.541%
13	8.037	2165	2176	2206	rBV	183828	385861	96.33%	11.213%
14	8.374	2270	2281	2288	rBV	5281	9872	2.46%	0.287%
15	8.792	2399	2411	2433	rBV	195089	343171	85.67%	9.972%
16	10.162	2825	2837	2852	rBV	73717	123154	30.74%	3.579%
17	10.333	2880	2890	2903	rVB2	20750	34813	8.69%	1.012%
18	11.194	3147	3158	3178	rBV	193838	310558	77.53%	9.024%
19	11.570	3260	3275	3291	rBV	167657	275067	68.67%	7.993%
20	12.207	3464	3473	3479	rBV6	4586	7397	1.85%	0.215%




Sum of corrected areas: 3441300

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030575.D
Acq On : 14 Apr 2023 15:58
Operator : SY/MD
Sample : 02275-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

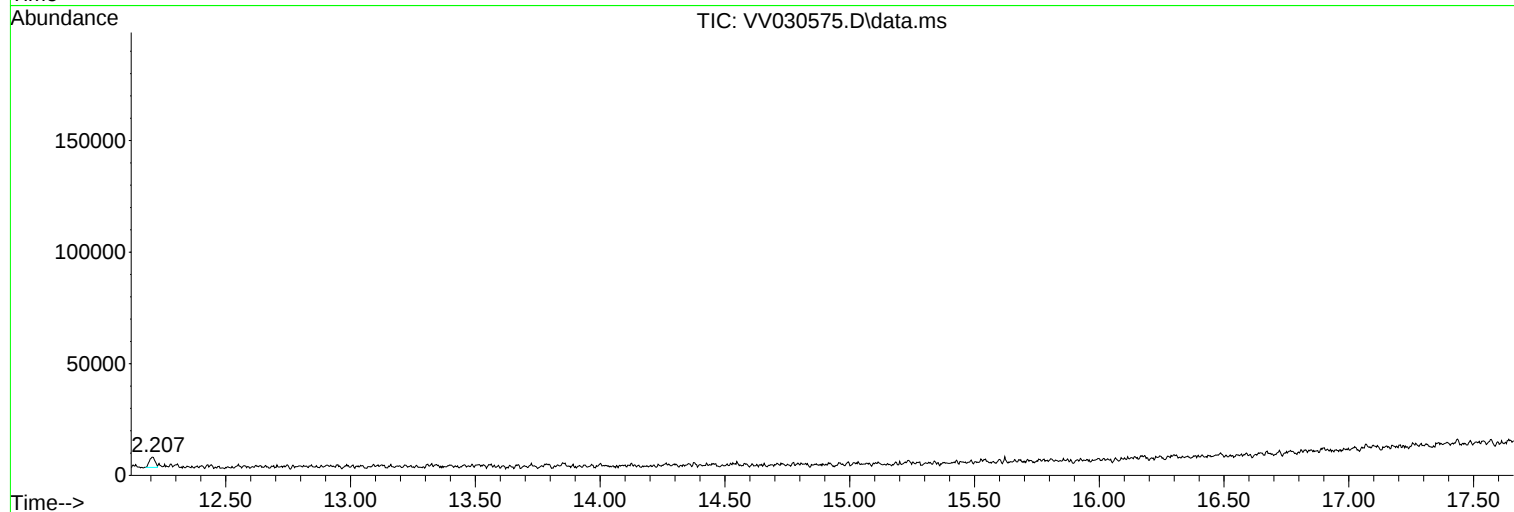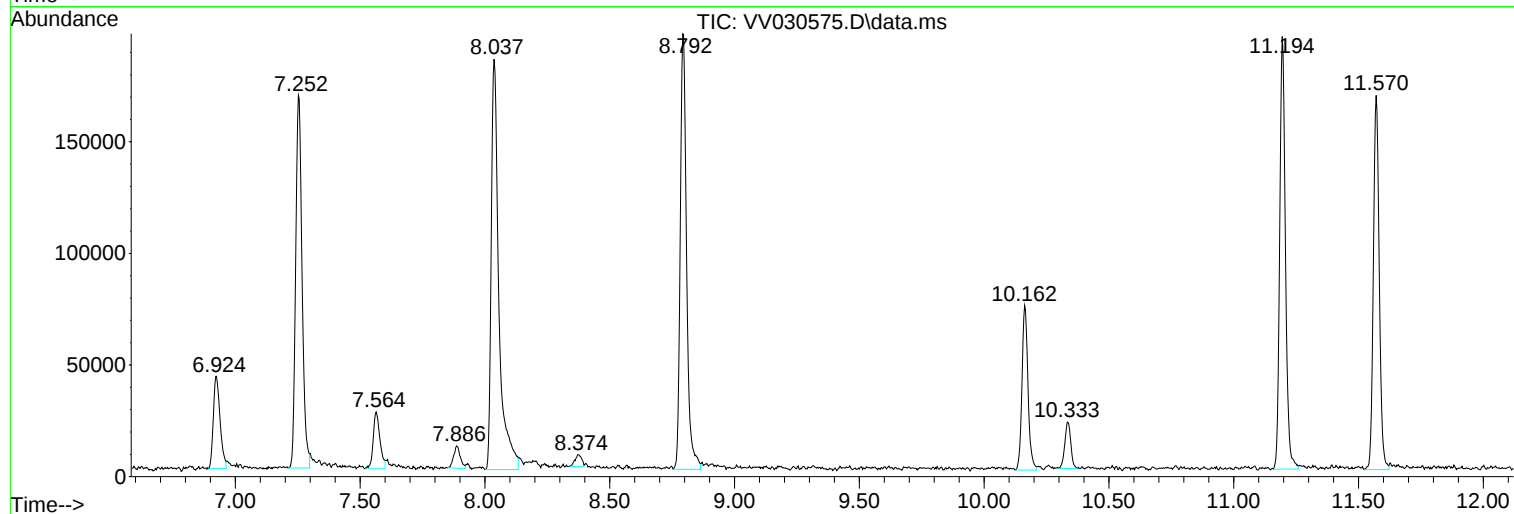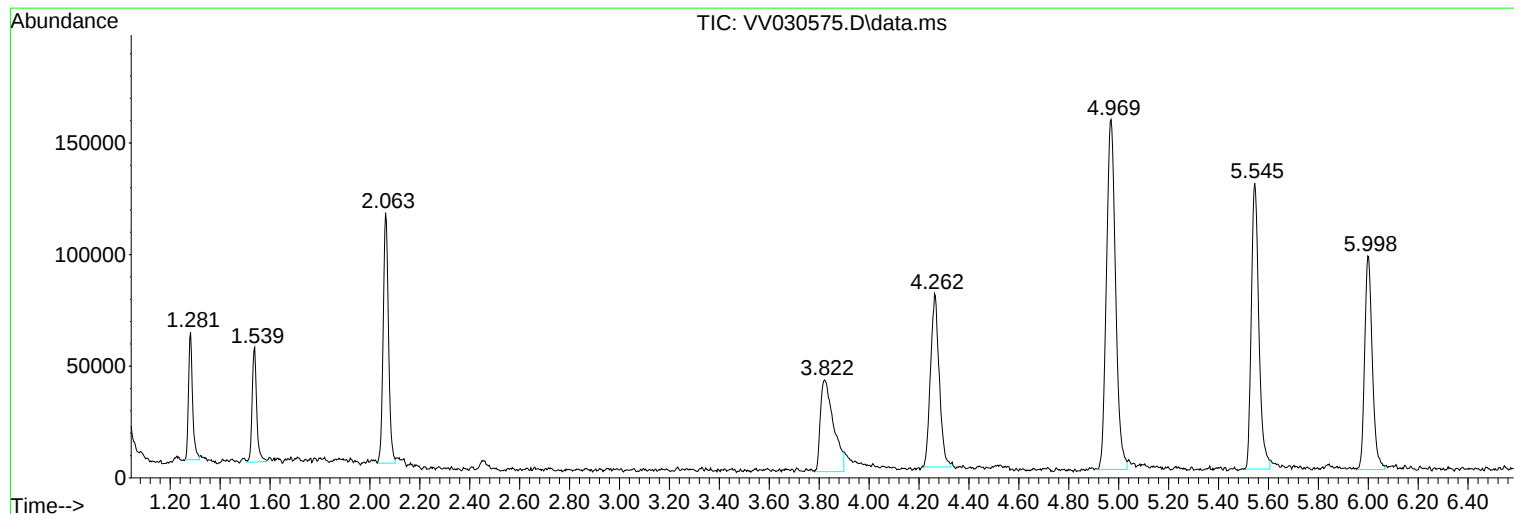

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030575.D
Acq On : 14 Apr 2023 15:58
Operator : SY/MD
Sample : 02275-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041423\
Data File : VV030575.D
Acq On : 14 Apr 2023 15:58
Operator : SY/MD
Sample : 02275-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc