

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041520\
 Data File : VV015523.D
 Acq On : 15 Apr 2020 21:02
 Operator : SY/MD
 Sample : L2274-24
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YAQE0

Quant Time: Apr 16 03:08:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 16 00:42:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	114198	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	106770	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	52690	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	28327	4.78	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.60%
7) Chloroethane-d5	1.58	69	26284	4.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.40%
11) 1,1-Dichloroethene-d2	2.12	63	41163	3.30	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.00%
20) 2-Butanone-d5	3.91	46	73591	44.23	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.46%
24) Chloroform-d	4.38	84	56874	4.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.60%
26) 1,2-Dichloroethane-d4	5.06	65	32803	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
32) Benzene-d6	5.08	84	114618	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
36) 1,2-Dichloropropane-d6	6.09	67	35423	4.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.00%
41) Toluene-d8	7.34	98	104359	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
43) trans-1,3-Dichloropropene-	7.65	79	13602	4.24	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.80%
46) 2-Hexanone-d5	8.11	63	58097	37.55	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.10%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	22932	3.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.40%
64) 1,2-Dichlorobenzene-d4	11.65	152	37344	4.42	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.40%


Target Compounds					Ovalue
13) Acetone	2.19	43	3037	2.584 ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV041520\
Data File : VV015523.D
Acq On : 15 Apr 2020 21:02
Operator : SY/MD
Sample : L2274-24
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YAE0

Quant Time: Apr 16 03:08:46 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 16 00:42:12 2020
Response via : Initial Calibration

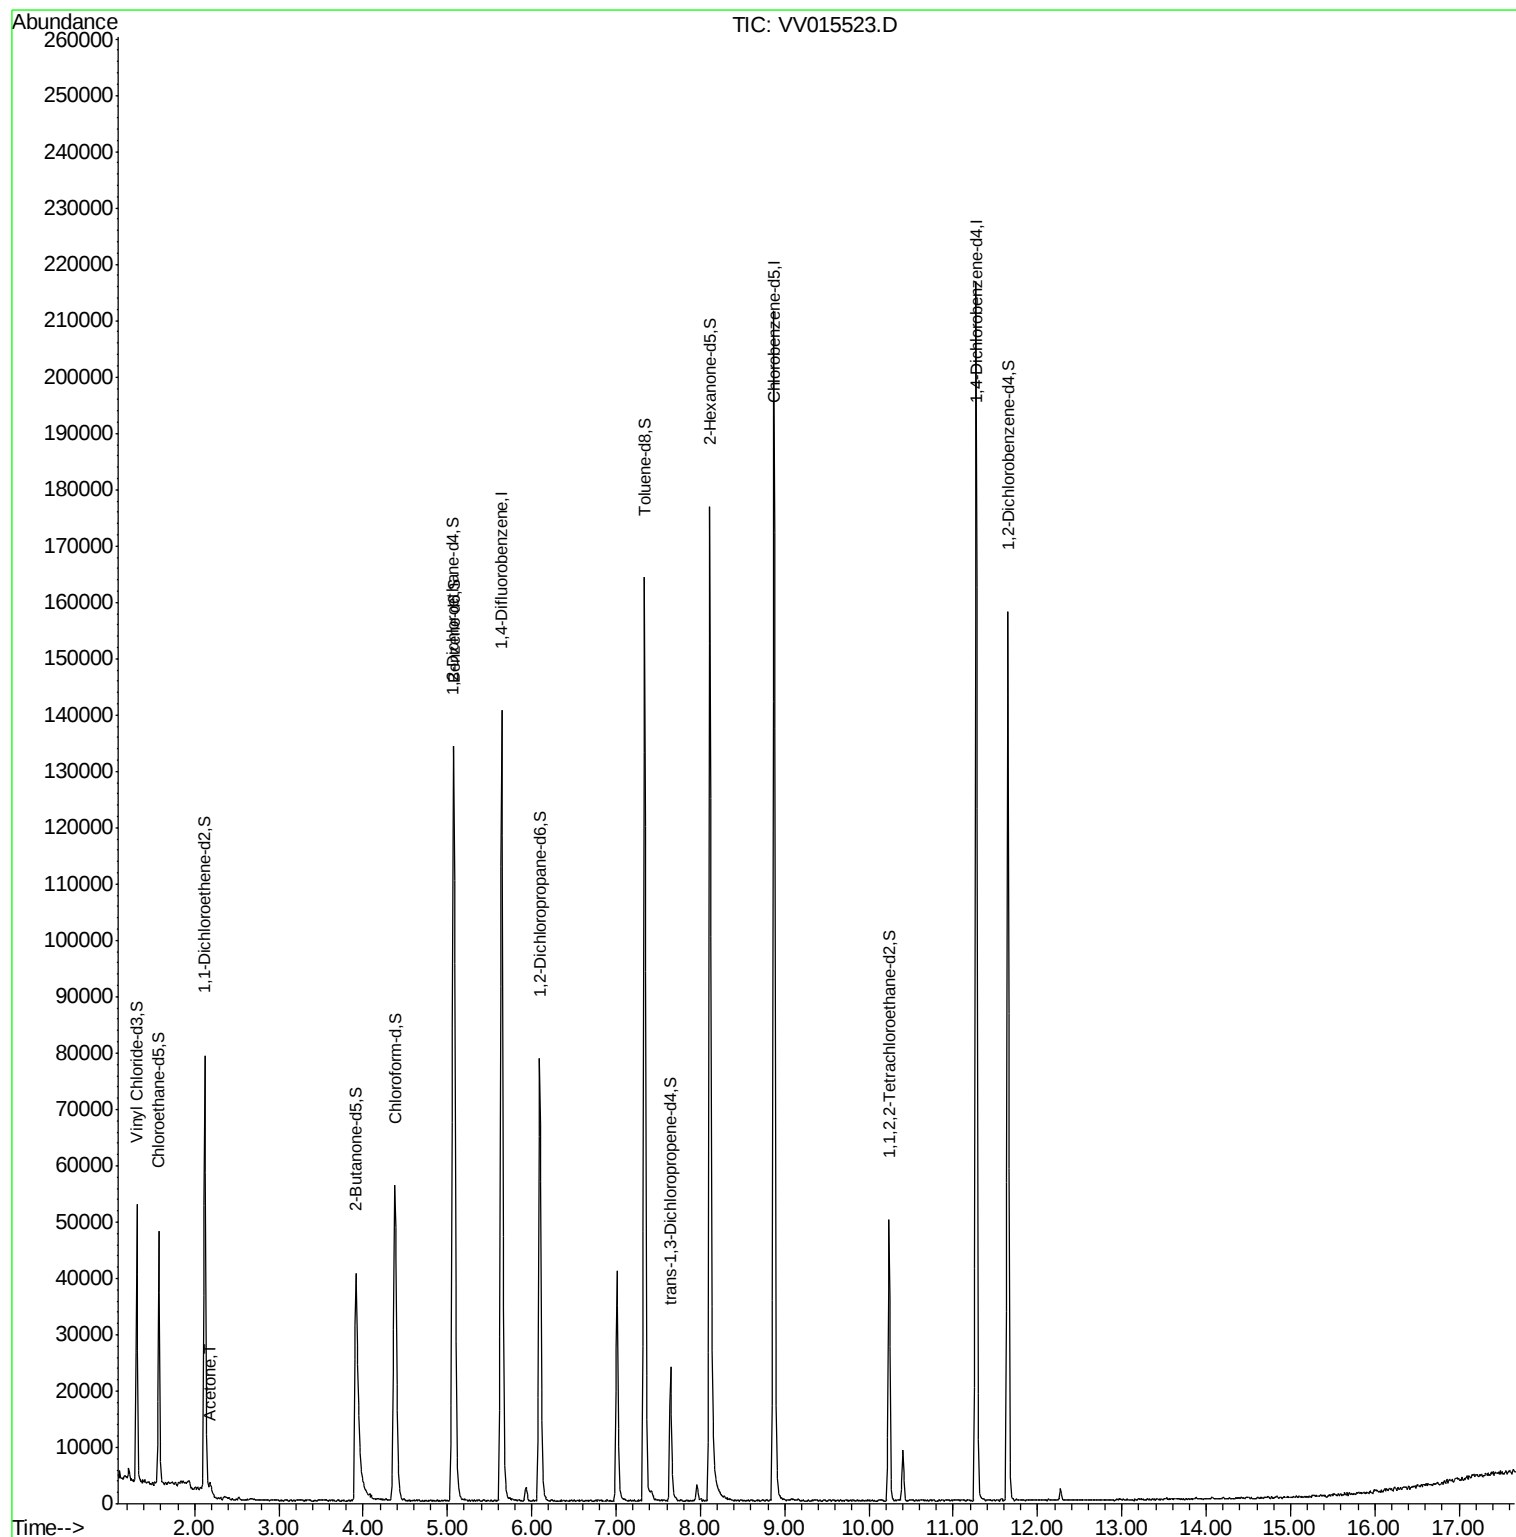

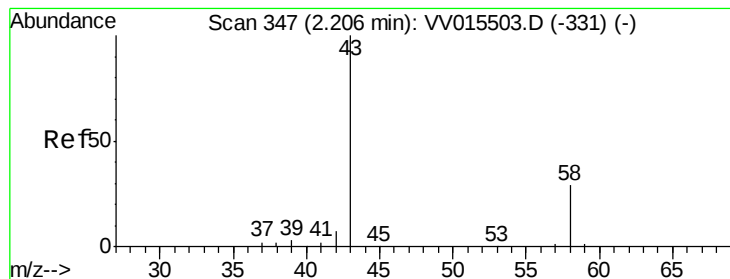

#13
 Acetone
 Concen: 2.584 ug/L
 RT: 2.19 min Scan# 342
 Delta R.T. -0.02 min
 Lab File: VV015523.D
 Acq: 15 Apr 2020 21:02

Instrument :
 MSVOA_V
 ClientSampleId :
 YAQE0

Tot Ion: 43 Resp: 3037
 Ion Ratio Lower Upper
 43 100
 58 23.0 0.0 22.2#

