


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV041520\
 Data File : VV015502.D
 Acq On : 15 Apr 2020 09:38
 Operator : SY/MD
 Sample : BFB35
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB35

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Apr 16 00:42:12 2020

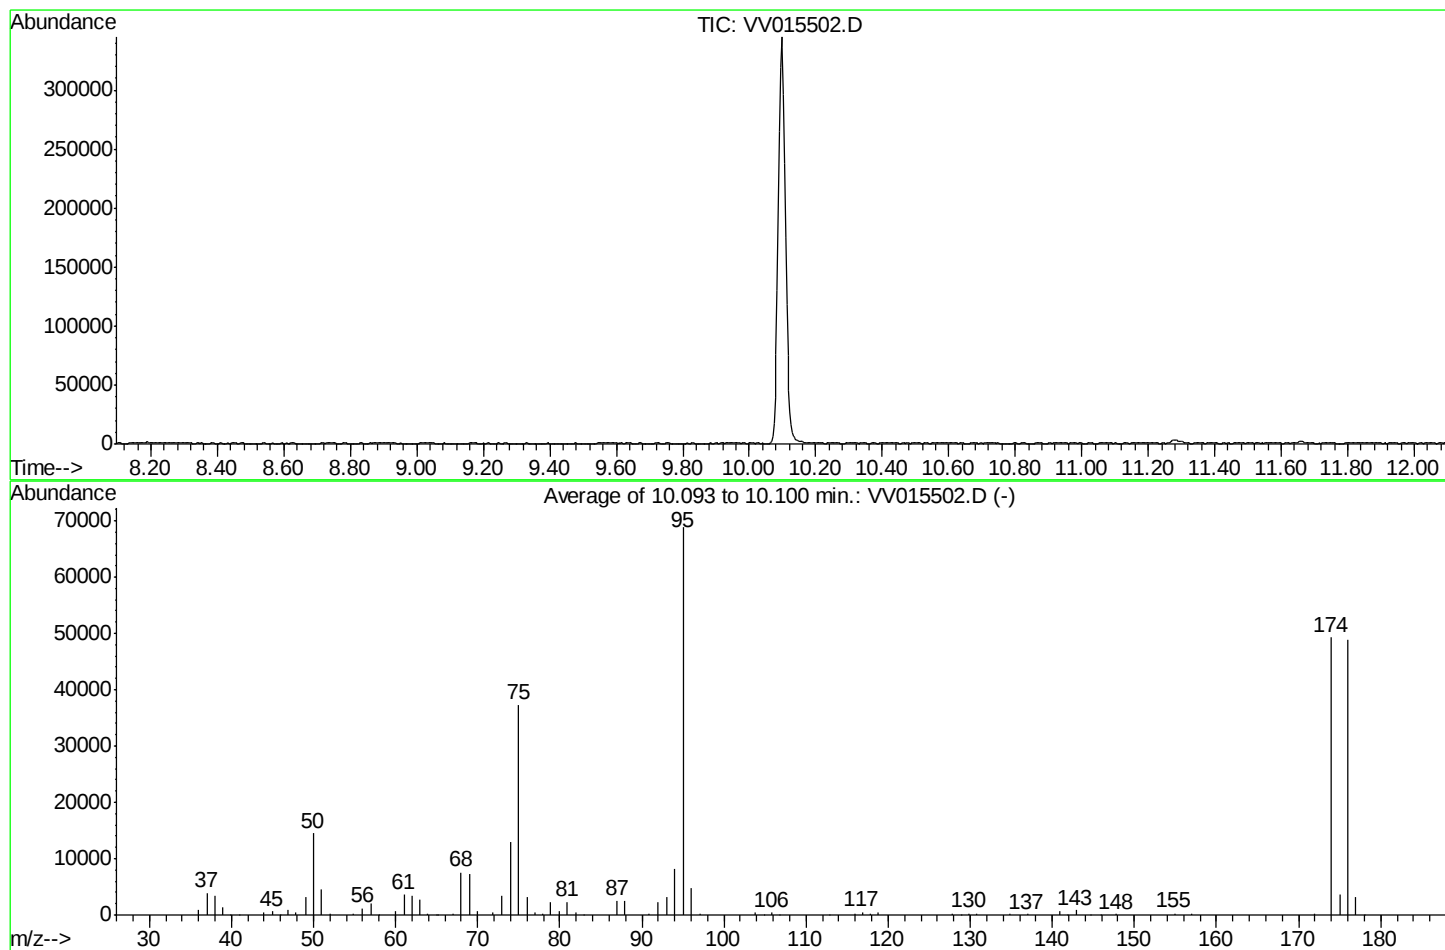

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	14519	PASS
75	95	30	80	54.3	37394	PASS
95	95	100	100	100.0	68850	PASS
96	95	5	9	6.9	4747	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.6	49306	PASS
175	174	5	9	7.6	3738	PASS
176	174	95	101	99.0	48797	PASS
177	176	5	9	6.4	3147	PASS

m/z	Abundance
36.00	882.0
37.00	3878.0
38.00	3378.0
39.00	1404.0
39.90	297.0
40.90	103.0
43.90	850.0
45.00	640.0
47.00	1023.0
47.90	486.0
49.00	3217.0
50.00	13968.0
51.00	4582.0
52.00	251.0
54.90	208.0
56.00	1220.0
57.00	2011.0
57.90	108.0
60.00	784.0
61.00	3464.0
62.00	3309.0
63.00	2643.0
64.00	233.0
65.00	126.0
66.90	214.0
68.00	7267.0
69.00	6982.0
70.00	624.0
71.90	468.0
73.00	3199.0
74.00	12615.0
75.00	36024.0
76.00	3148.0
76.90	378.0
77.90	326.0
78.90	2102.0
79.90	742.0
80.90	2283.0
81.90	528.0
87.00	2555.0
87.90	2364.0
90.90	291.0
92.00	2158.0
93.00	3140.0
94.00	7780.0
95.00	66048.0
96.00	4677.0
97.00	146.0
103.80	361.0
105.80	353.0
112.90	105.0
115.90	341.0
116.90	415.0
117.80	279.0
118.80	407.0
127.90	246.0
129.90	257.0
130.80	120.0
134.80	120.0
137.00	131.0
140.90	674.0
142.90	730.0
144.70	105.0
147.80	175.0
154.90	196.0
156.90	134.0
171.90	191.0
174.00	46400.0
175.00	3616.0
176.00	45280.0
177.00	3033.0
178.00	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
36.00	894.0
37.00	4054.0
38.00	3537.0
39.00	1500.0
39.90	306.0
43.90	837.0
45.00	687.0
47.00	1000.0
47.90	508.0
49.00	3295.0
50.00	15017.0
51.00	4696.0
52.00	247.0
54.90	255.0
56.00	1248.0
57.00	2048.0
57.90	115.0
60.00	767.0
61.00	3672.0
62.00	3571.0
63.00	2829.0
63.90	272.0
65.20	137.0
66.90	202.0
68.00	7832.0
69.00	7563.0
70.00	644.0
71.90	501.0
73.00	3391.0
74.00	13491.0
75.00	38736.0
76.00	3241.0
77.00	403.0
77.90	357.0
78.90	2241.0
79.90	780.0
80.90	2451.0
81.90	567.0
82.90	109.0
87.00	2717.0
87.90	2578.0
90.90	318.0
92.00	2333.0
93.00	3257.0
94.00	8410.0
95.00	71152.0
96.00	4952.0
97.10	162.0
103.80	359.0
104.80	112.0
105.90	398.0
112.90	104.0
115.90	372.0
116.90	502.0
117.80	300.0
118.80	428.0
127.80	281.0
128.90	121.0
129.90	292.0
130.80	133.0
134.80	134.0
136.90	121.0
140.90	683.0
141.80	105.0
142.90	832.0
144.70	104.0
145.90	118.0
147.80	237.0
154.90	247.0
156.90	151.0
171.90	216.0
174.00	50896.0
175.00	3847.0
176.00	50608.0
177.00	3277.0
178.00	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
36.00	774.0
37.00	3902.0
38.00	3279.0
39.00	1460.0
39.90	320.0
43.90	779.0
45.00	651.0
46.00	105.0
46.90	918.0
47.90	481.0
49.00	3066.0
50.00	14572.0
51.00	4327.0
52.00	225.0
54.90	277.0
56.00	1200.0
57.00	1925.0
58.00	117.0
60.00	668.0
61.00	3531.0
62.00	3422.0
63.00	2724.0
63.90	312.0
65.20	132.0
67.00	176.0
68.00	7613.0
69.00	7377.0
70.00	644.0
71.90	468.0
73.00	3373.0
74.00	12950.0
75.00	37424.0
76.00	3068.0
77.00	428.0
78.00	332.0
78.90	2211.0
79.90	723.0
80.90	2367.0
81.90	531.0
82.90	103.0
87.00	2545.0
88.00	2523.0
90.90	305.0
92.00	2208.0
93.00	2998.0
94.00	8156.0
95.00	69352.0
96.00	4612.0
97.00	161.0
103.80	336.0
104.90	110.0
105.90	396.0
106.80	125.0
115.90	337.0
116.90	535.0
117.80	300.0
118.80	412.0
127.80	301.0
128.90	124.0
129.90	287.0
130.80	124.0
134.80	141.0
136.90	148.0
140.90	701.0
141.80	106.0
142.90	883.0
145.90	126.0
147.80	261.0
154.90	256.0
157.00	139.0
171.90	213.0
174.00	50624.0
175.00	3752.0
176.00	50504.0
177.00	3131.0
178.00	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

Scan 2788 (10.055 min): VV015502.D
BFB35

m/z	Abundance
39.90	265.0
44.00	279.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35