

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041521\
 Data File : VV021030.D
 Acq On : 15 Apr 2021 15:22
 Operator : SY/MD
 Sample : M2031-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG541

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M

Title : VOC Analysis

Signal : TIC: VV021030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	78	84	100	rVB	167096	186706	11.42%	1.452%
2	1.571	159	165	179	rVB	143231	181153	11.08%	1.409%
3	2.108	323	332	350	rBV	373071	531832	32.52%	4.136%
4	2.381	414	417	419	rBV2	653	458	0.03%	0.004%
5	2.420	426	429	436	rBV3	686	796	0.05%	0.006%
6	2.558	469	472	474	rBV3	488	406	0.02%	0.003%
7	2.651	499	501	505	rBV	591	396	0.02%	0.003%
8	2.732	524	526	530	rBV2	407	323	0.02%	0.003%
9	2.973	597	601	605	rVB3	401	340	0.02%	0.003%
10	3.262	687	691	693	rBV	394	345	0.02%	0.003%
11	3.384	727	729	732	rVV2	576	328	0.02%	0.003%
12	3.551	779	781	786	rVB3	587	312	0.02%	0.002%
13	3.638	806	808	815	rBV2	522	612	0.04%	0.005%
14	3.683	819	822	826	rVB	459	323	0.02%	0.003%
15	3.725	831	835	836	rBV2	582	351	0.02%	0.003%
16	3.828	865	867	871	rVB3	577	388	0.02%	0.003%
17	3.908	881	892	932	rBV2	71772	280457	17.15%	2.181%
18	4.352	1015	1030	1061	rBV	288922	719532	44.00%	5.595%
19	4.532	1082	1086	1089	rBV2	951	710	0.04%	0.006%
20	4.725	1140	1146	1147	rBV2	785	613	0.04%	0.005%
21	4.895	1195	1199	1204	rBV3	347	403	0.02%	0.003%
22	5.050	1231	1247	1274	rBV2	631328	1635416	100.00%	12.718%
23	5.252	1308	1310	1314	rVB	733	359	0.02%	0.003%
24	5.272	1314	1316	1319	rBV3	860	431	0.03%	0.003%
25	5.394	1351	1354	1358	rBV4	801	698	0.04%	0.005%
26	5.542	1398	1400	1402	rVB	673	326	0.02%	0.003%
27	5.567	1402	1408	1409	rBV	673	557	0.03%	0.004%
28	5.622	1413	1425	1450	rBV	538924	1083126	66.23%	8.423%
29	5.857	1496	1498	1501	rBV3	693	434	0.03%	0.003%
30	5.960	1529	1530	1532	rBV3	537	298	0.02%	0.002%
31	6.075	1552	1566	1591	rBV	346937	710147	43.42%	5.522%
32	6.371	1654	1658	1661	rVB2	737	472	0.03%	0.004%
33	6.490	1691	1695	1696	rBV	419	325	0.02%	0.003%
34	6.580	1718	1723	1726	rBV2	927	847	0.05%	0.007%
35	6.702	1758	1761	1765	rVV2	464	418	0.03%	0.003%
36	6.854	1803	1808	1811	rVV3	384	314	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041521\
 Data File : VV021030.D
 Acq On : 15 Apr 2021 15:22
 Operator : SY/MD
 Sample : M2031-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG541

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.899	1820	1822	1830	rVB4	617	618	0.04%	0.005%
38	6.940	1832	1835	1838	rBV2	925	617	0.04%	0.005%
39	6.989	1840	1850	1876	rVV	211688	381944	23.35%	2.970%
40	7.175	1907	1908	1913	rVB3	617	305	0.02%	0.002%
41	7.243	1927	1929	1931	rBV	656	448	0.03%	0.003%
42	7.320	1940	1953	1970	rBV	796859	1363059	83.35%	10.600%
43	7.625	2038	2048	2070	rBV	145650	258130	15.78%	2.007%
44	7.944	2134	2147	2148	rBV7	3744	4496	0.27%	0.035%
45	8.005	2162	2166	2174	rBV3	746	1033	0.06%	0.008%
46	8.095	2184	2194	2223	rBV	372370	669335	40.93%	5.205%
47	8.355	2272	2275	2276	rBV3	695	399	0.02%	0.003%
48	8.500	2318	2320	2324	rVB3	667	326	0.02%	0.003%
49	8.526	2324	2328	2332	rBV3	569	633	0.04%	0.005%
50	8.571	2339	2342	2346	rBV2	540	422	0.03%	0.003%
51	8.673	2370	2374	2376	rBV	384	325	0.02%	0.003%
52	8.857	2418	2431	2455	rBV	823903	1316757	80.52%	10.240%
53	9.136	2514	2518	2519	rBV2	1483	757	0.05%	0.006%
54	9.349	2582	2584	2589	rBV2	572	366	0.02%	0.003%
55	9.403	2599	2601	2605	rVB2	438	288	0.02%	0.002%
56	9.435	2605	2611	2612	rBV2	379	281	0.02%	0.002%
57	9.468	2619	2621	2626	rVB	486	342	0.02%	0.003%
58	9.535	2638	2642	2643	rBV2	452	286	0.02%	0.002%
59	9.683	2685	2688	2692	rBV2	452	428	0.03%	0.003%
60	9.792	2718	2722	2726	rVB2	515	329	0.02%	0.003%
61	9.853	2738	2741	2743	rBV2	466	335	0.02%	0.003%
62	9.947	2767	2770	2778	rVB3	702	834	0.05%	0.006%
63	9.979	2778	2780	2785	rBV3	425	314	0.02%	0.002%
64	10.017	2790	2792	2796	rVV2	488	316	0.02%	0.002%
65	10.088	2812	2814	2817	rBV2	566	382	0.02%	0.003%
66	10.223	2843	2856	2877	rBV	564591	879792	53.80%	6.842%
67	10.387	2898	2907	2916	rVB6	3490	5934	0.36%	0.046%
68	10.432	2919	2921	2926	rBV3	680	505	0.03%	0.004%
69	10.509	2942	2945	2949	rBV2	642	612	0.04%	0.005%
70	10.542	2953	2955	2961	rBV2	639	493	0.03%	0.004%
71	10.574	2963	2965	2966	rBV2	708	324	0.02%	0.003%
72	10.670	2992	2995	3000	rBV	597	453	0.03%	0.004%
73	10.841	3043	3048	3050	rBV2	519	498	0.03%	0.004%
74	10.927	3068	3075	3088	rVB9	3578	6140	0.38%	0.048%
75	10.982	3088	3092	3095	rBV	574	415	0.03%	0.003%
76	11.037	3105	3109	3111	rBV2	746	489	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041521\
 Data File : VV021030.D
 Acq On : 15 Apr 2021 15:22
 Operator : SY/MD
 Sample : M2031-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG541

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	11.255	3165	3177	3198	rBV	804280	1249981	76.43%	9.720%
78	11.509	3252	3256	3257	rBV2	1504	953	0.06%	0.007%
79	11.631	3282	3294	3313	rBV	862159	1357432	83.00%	10.556%
80	11.786	3340	3342	3345	rVB3	1030	613	0.04%	0.005%
81	11.924	3382	3385	3387	rBV4	517	297	0.02%	0.002%
82	12.027	3415	3417	3420	rVB2	820	361	0.02%	0.003%
83	12.049	3420	3424	3427	rBV2	364	404	0.02%	0.003%
84	12.075	3430	3432	3434	rBV	689	290	0.02%	0.002%
85	12.210	3470	3474	3476	rBV2	543	495	0.03%	0.004%
86	12.246	3481	3485	3486	rBV2	791	561	0.03%	0.004%
87	12.278	3492	3495	3499	rVB3	1223	992	0.06%	0.008%
88	12.397	3530	3532	3535	rBV2	506	377	0.02%	0.003%
89	12.445	3545	3547	3555	rVB2	698	670	0.04%	0.005%
90	12.789	3651	3654	3657	rBV2	454	326	0.02%	0.003%
91	12.850	3671	3673	3675	rBV2	552	278	0.02%	0.002%
92	13.049	3732	3735	3739	rBV3	484	312	0.02%	0.002%
93	13.075	3739	3743	3746	rBV2	473	370	0.02%	0.003%
94	13.098	3748	3750	3754	rBV2	482	374	0.02%	0.003%
95	13.175	3771	3774	3777	rBV2	760	516	0.03%	0.004%
96	13.429	3850	3853	3856	rVB	760	456	0.03%	0.004%
97	13.564	3893	3895	3896	rBV	645	290	0.02%	0.002%
98	13.760	3952	3956	3960	rVB2	921	676	0.04%	0.005%
99	14.004	4028	4032	4041	rBV3	866	1284	0.08%	0.010%
100	14.268	4111	4114	4115	rBV	536	290	0.02%	0.002%




Sum of corrected areas: 12859310

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041521\
Data File : VV021030.D
Acq On : 15 Apr 2021 15:22
Operator : SY/MD
Sample : M2031-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG541

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

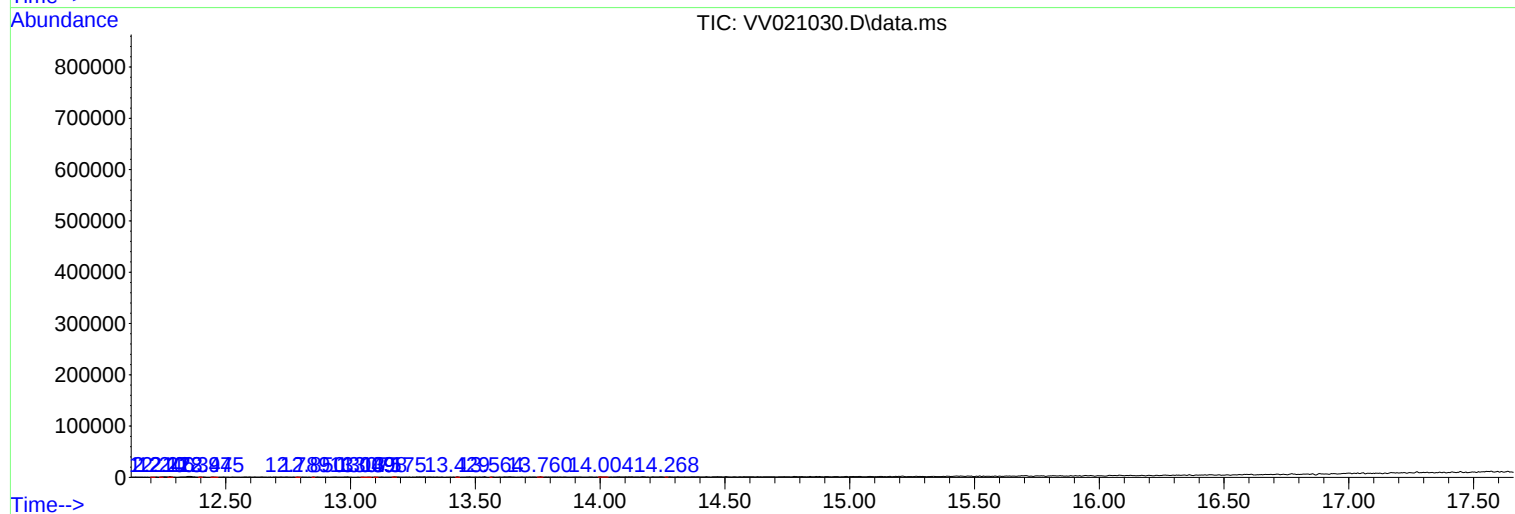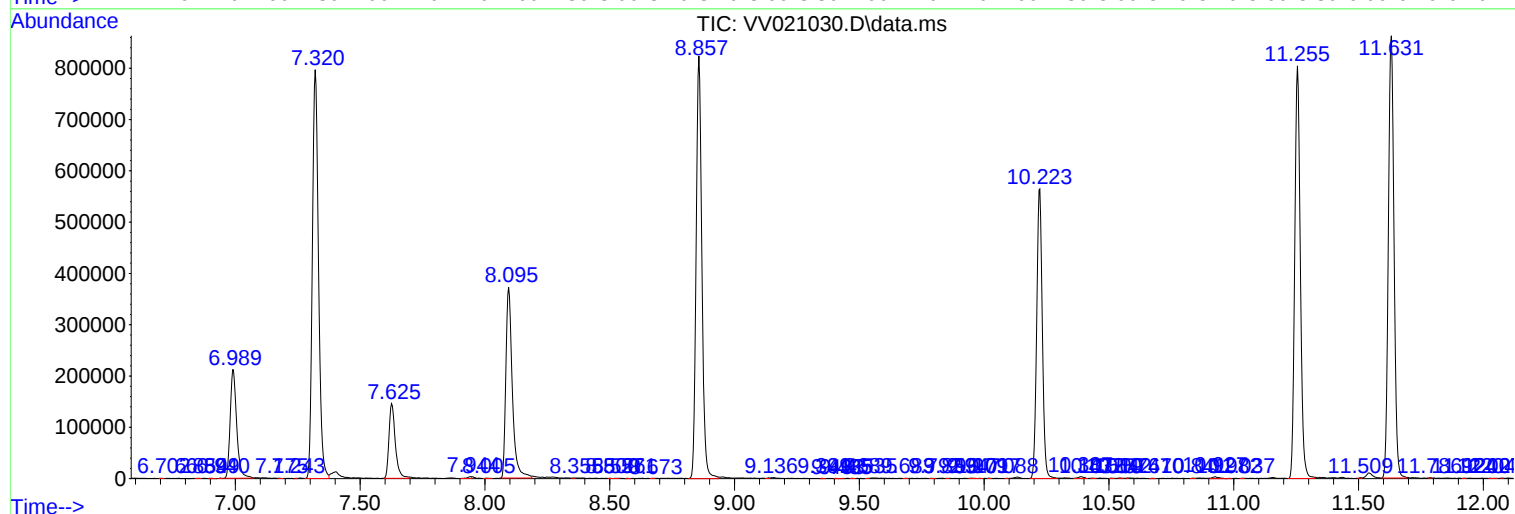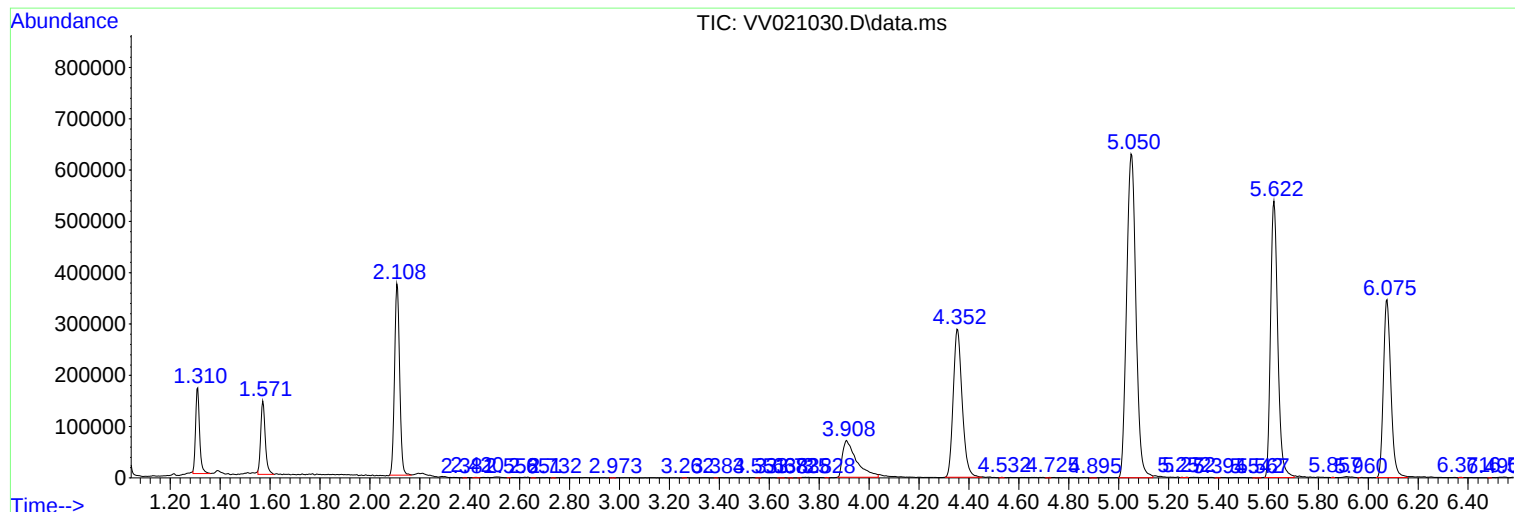

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041521\
Data File : VV021030.D
Acq On : 15 Apr 2021 15:22
Operator : SY/MD
Sample : M2031-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG541

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041521\
Data File : VV021030.D
Acq On : 15 Apr 2021 15:22
Operator : SY/MD
Sample : M2031-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG541

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
