

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041521\
 Data File : VV021034.D
 Acq On : 15 Apr 2021 16:59
 Operator : SY/MD
 Sample : M2062-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

Signal : TIC: VV021034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	102	rVB	158705	182945	10.98%	1.399%
2	1.571	158	165	181	rVB	140995	181931	10.92%	1.391%
3	2.108	323	332	344	rBV	380665	538612	32.31%	4.119%
4	2.294	387	390	398	rVB3	2164	2225	0.13%	0.017%
5	2.394	419	421	424	rVB2	483	231	0.01%	0.002%
6	2.654	500	502	505	rVB	569	207	0.01%	0.002%
7	2.777	538	540	542	rBV	396	258	0.02%	0.002%
8	2.934	586	589	593	rVB	411	291	0.02%	0.002%
9	2.953	593	595	601	rBV2	492	422	0.03%	0.003%
10	3.037	618	621	626	rVV2	592	518	0.03%	0.004%
11	3.098	636	640	643	rBV2	278	260	0.02%	0.002%
12	3.159	655	659	660	rBV	509	254	0.02%	0.002%
13	3.262	687	691	694	rBV2	457	396	0.02%	0.003%
14	3.326	708	711	713	rBV2	461	213	0.01%	0.002%
15	3.397	730	733	736	rBV3	366	269	0.02%	0.002%
16	3.439	739	746	749	rBV2	390	483	0.03%	0.004%
17	3.458	749	752	754	rBV2	491	304	0.02%	0.002%
18	3.529	771	774	776	rBV	473	293	0.02%	0.002%
19	3.561	781	784	786	rBV2	504	335	0.02%	0.003%
20	3.834	865	869	871	rBV	555	499	0.03%	0.004%
21	3.857	874	876	881	rVB2	433	309	0.02%	0.002%
22	3.908	881	892	932	rBV2	84523	309758	18.58%	2.369%
23	4.355	1015	1031	1058	rBV2	287606	735659	44.14%	5.626%
24	4.535	1085	1087	1089	rBV	431	258	0.02%	0.002%
25	4.674	1128	1130	1132	rBV2	569	323	0.02%	0.002%
26	4.709	1139	1141	1146	rVB4	774	442	0.03%	0.003%
27	4.735	1146	1149	1150	rBV2	292	200	0.01%	0.002%
28	4.799	1163	1169	1173	rBV	695	643	0.04%	0.005%
29	4.889	1192	1197	1202	rBV2	259	272	0.02%	0.002%
30	4.918	1202	1206	1209	rBV2	411	258	0.02%	0.002%
31	4.934	1209	1211	1216	rVB2	605	473	0.03%	0.004%
32	5.050	1229	1247	1277	rBV2	649386	1666775	100.00%	12.747%
33	5.394	1351	1354	1356	rBV2	558	365	0.02%	0.003%
34	5.432	1364	1366	1367	rBV2	570	232	0.01%	0.002%
35	5.481	1376	1381	1383	rBV3	690	540	0.03%	0.004%
36	5.561	1401	1406	1407	rBV2	444	257	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041521\
 Data File : VV021034.D
 Acq On : 15 Apr 2021 16:59
 Operator : SY/MD
 Sample : M2062-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	5.622	1412	1425	1454	rBV	536443	1073681	64.42%	8.211%
38	5.947	1524	1526	1529	rVB2	700	347	0.02%	0.003%
39	6.075	1552	1566	1590	rBV	356266	726957	43.61%	5.560%
40	6.268	1623	1626	1628	rBV3	460	330	0.02%	0.003%
41	6.297	1632	1635	1640	rVB3	892	853	0.05%	0.007%
42	6.323	1640	1643	1645	rBV	706	483	0.03%	0.004%
43	6.387	1658	1663	1664	rBV	558	371	0.02%	0.003%
44	6.429	1674	1676	1681	rVB2	640	578	0.03%	0.004%
45	6.455	1681	1684	1687	rBV	321	253	0.02%	0.002%
46	6.493	1692	1696	1698	rBV	557	362	0.02%	0.003%
47	6.551	1710	1714	1715	rBV2	468	274	0.02%	0.002%
48	6.603	1727	1730	1735	rVB2	611	484	0.03%	0.004%
49	6.693	1756	1758	1763	rVB3	497	377	0.02%	0.003%
50	6.722	1763	1767	1769	rBV	523	273	0.02%	0.002%
51	6.741	1772	1773	1775	rBV	375	208	0.01%	0.002%
52	6.860	1804	1810	1812	rBV2	502	454	0.03%	0.003%
53	6.992	1839	1851	1867	rBV	216349	385469	23.13%	2.948%
54	7.272	1936	1938	1941	rVB	626	242	0.01%	0.002%
55	7.320	1941	1953	1970	rBV	784316	1363176	81.79%	10.425%
56	7.577	2031	2033	2035	rBV	371	208	0.01%	0.002%
57	7.625	2038	2048	2069	rBV	152291	267624	16.06%	2.047%
58	7.805	2098	2104	2111	rBV4	950	1480	0.09%	0.011%
59	7.850	2115	2118	2120	rBV	449	324	0.02%	0.002%
60	7.927	2137	2142	2143	rBV2	850	624	0.04%	0.005%
61	8.021	2169	2171	2174	rVB2	667	276	0.02%	0.002%
62	8.095	2184	2194	2218	rBV	419239	728629	43.71%	5.572%
63	8.432	2294	2299	2302	rBV4	1059	798	0.05%	0.006%
64	8.529	2327	2329	2334	rVV2	563	375	0.02%	0.003%
65	8.728	2388	2391	2393	rBV2	412	227	0.01%	0.002%
66	8.857	2419	2431	2451	rBV	826101	1310335	78.61%	10.021%
67	9.130	2513	2516	2520	rBV2	798	719	0.04%	0.005%
68	9.159	2520	2525	2526	rBV3	938	819	0.05%	0.006%
69	9.194	2534	2536	2539	rVB2	560	251	0.02%	0.002%
70	9.217	2541	2543	2546	rVV	735	416	0.02%	0.003%
71	9.252	2550	2554	2558	rVB3	410	288	0.02%	0.002%
72	9.419	2603	2606	2611	rBV3	622	541	0.03%	0.004%
73	9.567	2646	2652	2655	rBV2	566	654	0.04%	0.005%
74	9.722	2698	2700	2703	rBV2	438	294	0.02%	0.002%
75	9.757	2708	2711	2716	rVB2	489	468	0.03%	0.004%
76	9.841	2734	2737	2738	rBV2	401	247	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041521\
 Data File : VV021034.D
 Acq On : 15 Apr 2021 16:59
 Operator : SY/MD
 Sample : M2062-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	9.937	2765	2767	2768	rBV	485	229	0.01%	0.002%
78	10.024	2792	2794	2797	rVB2	689	356	0.02%	0.003%
79	10.053	2800	2803	2806	rBV2	449	354	0.02%	0.003%
80	10.220	2844	2855	2877	rBV	591817	920610	55.23%	7.041%
81	10.535	2950	2953	2955	rBV2	257	206	0.01%	0.002%
82	10.548	2955	2957	2959	rBV	476	266	0.02%	0.002%
83	10.673	2994	2996	3000	rBV	302	222	0.01%	0.002%
84	10.850	3049	3051	3054	rBV2	705	465	0.03%	0.004%
85	10.921	3068	3073	3075	rBV3	2236	1862	0.11%	0.014%
86	10.976	3088	3090	3093	rBV	425	303	0.02%	0.002%
87	10.988	3093	3094	3098	rVB2	495	307	0.02%	0.002%
88	11.146	3139	3143	3150	rBV4	1784	2119	0.13%	0.016%
89	11.255	3166	3177	3199	rBV	818566	1256602	75.39%	9.610%
90	11.532	3260	3263	3266	rBV2	490	410	0.02%	0.003%
91	11.631	3280	3294	3315	rBV	889810	1388886	83.33%	10.622%
92	12.091	3433	3437	3438	rBV	727	445	0.03%	0.003%
93	12.181	3462	3465	3469	rBV2	423	413	0.02%	0.003%
94	12.262	3487	3490	3493	rVB	1238	747	0.04%	0.006%
95	12.332	3510	3512	3514	rBV	497	219	0.01%	0.002%
96	12.770	3645	3648	3649	rBV	568	319	0.02%	0.002%
97	13.117	3754	3756	3759	rBV	520	348	0.02%	0.003%
98	13.715	3939	3942	3945	rBV2	809	579	0.03%	0.004%
99	14.310	4125	4127	4129	rBV3	978	576	0.03%	0.004%
100	14.528	4193	4195	4197	rBV2	763	357	0.02%	0.003%




Sum of corrected areas: 13075679

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041521\
Data File : VV021034.D
Acq On : 15 Apr 2021 16:59
Operator : SY/MD
Sample : M2062-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

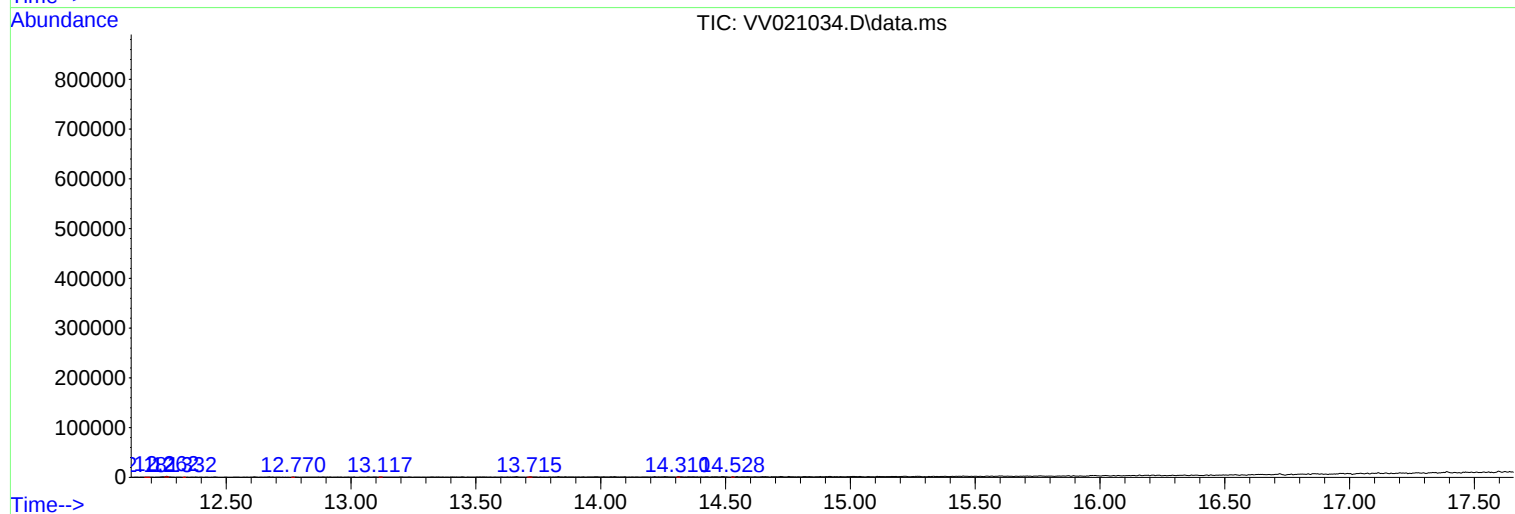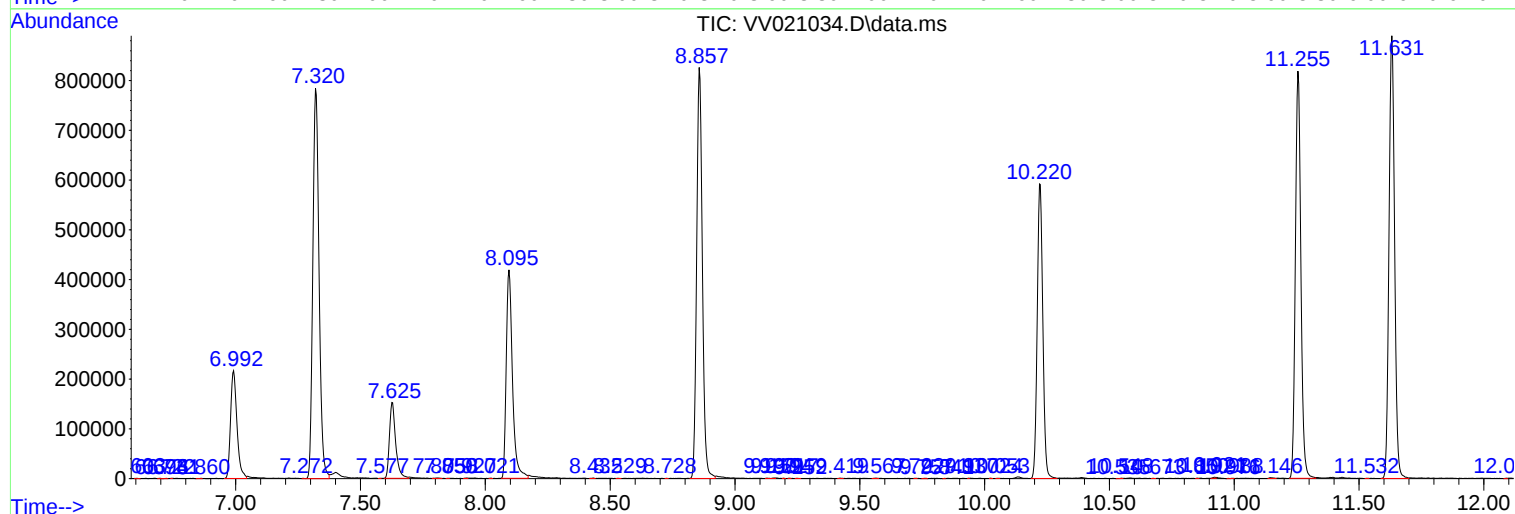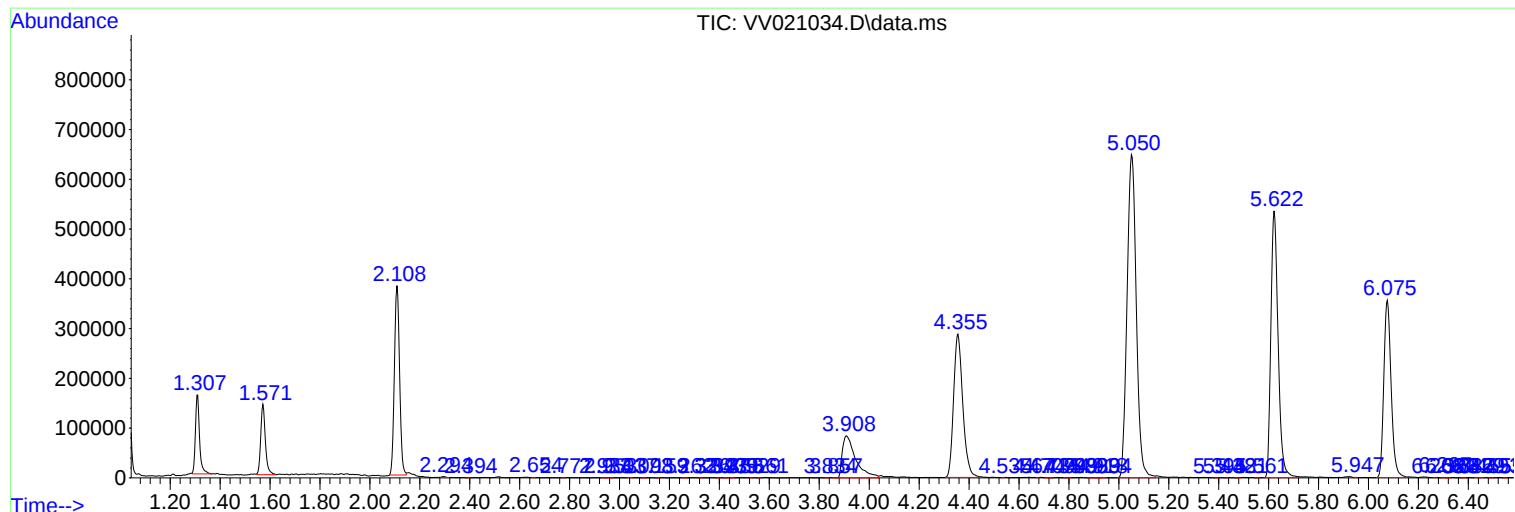

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041521\
Data File : VV021034.D
Acq On : 15 Apr 2021 16:59
Operator : SY/MD
Sample : M2062-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041521\
Data File : VV021034.D
Acq On : 15 Apr 2021 16:59
Operator : SY/MD
Sample : M2062-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
