
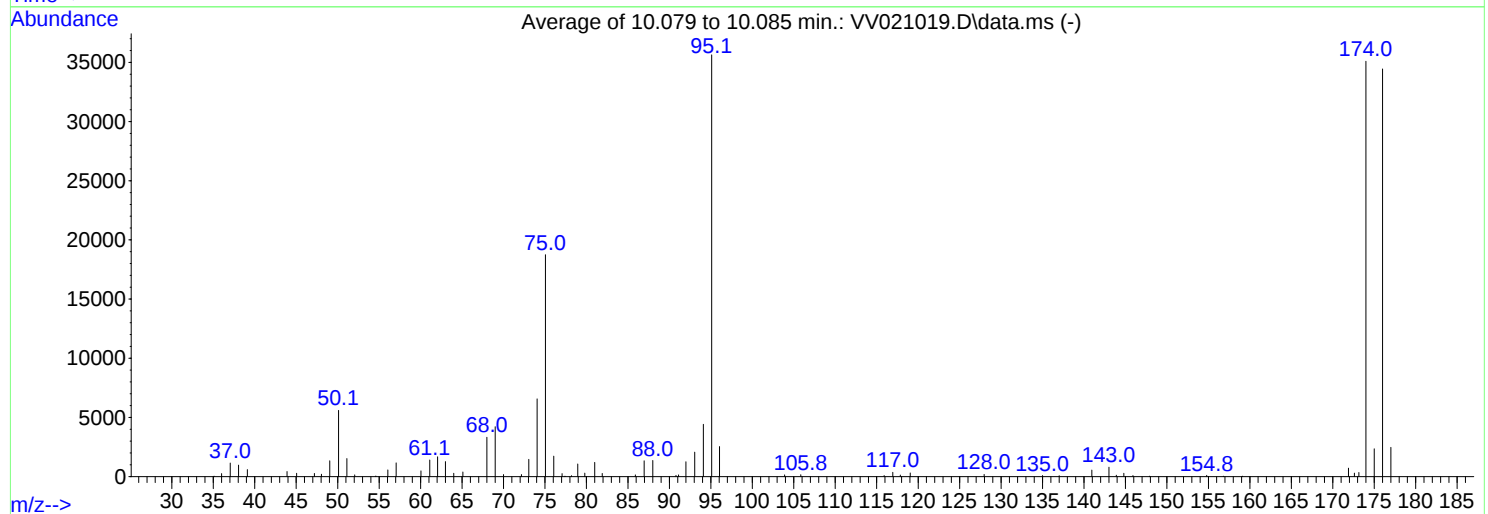


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041521\
 Data File : VV021019.D
 Acq On : 15 Apr 2021 09:06
 Operator : SY/MD
 Sample : BFB83
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB832

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis
 Last Update : Sat Apr 17 00:47:19 2021

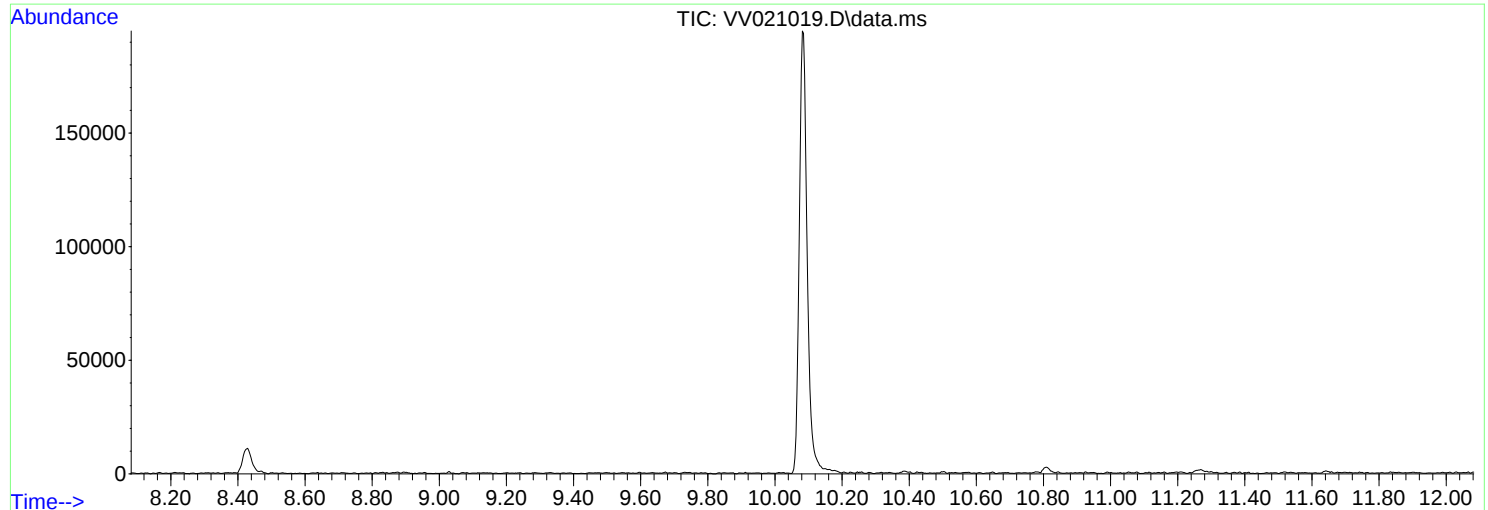

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	5600	PASS
75	95	30	80	52.6	18752	PASS
95	95	100	100	100.0	35635	PASS
96	95	5	9	7.1	2537	PASS
173	174	0.00	2	1.0	356	PASS
174	95	50	120	98.5	35091	PASS
175	174	5	9	6.7	2357	PASS
176	174	95	101	98.2	34445	PASS
177	176	5	9	7.2	2471	PASS

m/z	Abundance
36.00	316.0
37.10	1234.0
38.10	892.0
39.10	650.0
40.00	272.0
43.90	362.0
45.00	312.0
47.20	349.0
48.00	181.0
49.10	1271.0
50.10	5160.0
51.10	1460.0
52.00	142.0
54.60	156.0
56.00	528.0
57.10	1003.0
60.00	514.0
61.00	1200.0
62.10	1752.0
63.00	1275.0
63.90	336.0
65.10	389.0
68.00	3687.0
69.00	4315.0
70.00	197.0
72.20	175.0
73.10	1680.0
74.00	7011.0
75.10	18928.0
76.10	1829.0
77.10	310.0
78.20	231.0
79.00	1019.0
79.80	354.0
81.00	1322.0
81.90	290.0
85.90	264.0
87.00	1370.0
88.00	1324.0
90.80	178.0
91.10	177.0
92.00	1164.0
93.00	2069.0
94.10	4617.0
95.10	36424.0
96.10	2497.0
103.90	166.0
105.80	136.0
115.90	166.0
116.90	427.0
117.80	158.0
119.10	278.0
127.90	181.0
135.00	133.0
141.00	523.0
143.00	828.0
143.90	109.0
144.80	261.0
147.90	114.0
156.80	117.0
171.90	818.0
173.10	598.0
174.00	36200.0
175.00	2510.0
176.00	36448.0
177.00	2454.0

Instrument :
MSVOA_V
ClientSampleId :
BFB832

m/z	Abundance
36.00	240.0
37.00	1203.0
38.00	967.0
39.10	609.0
40.00	222.0
43.90	435.0
45.00	299.0
47.20	274.0
48.10	207.0
49.00	1401.0
50.10	5883.0
51.10	1523.0
52.00	171.0
56.10	577.0
57.10	1272.0
60.00	494.0
61.10	1453.0
62.10	1774.0
63.00	1259.0
64.00	286.0
65.10	408.0
68.00	3460.0
69.00	4391.0
70.00	184.0
72.10	169.0
73.10	1473.0
74.10	6890.0
75.10	19544.0
76.00	1783.0
77.00	242.0
78.90	1127.0
79.80	309.0
81.00	1217.0
81.90	266.0
85.90	195.0
87.00	1370.0
88.00	1452.0
90.80	145.0
91.10	158.0
92.00	1305.0
93.00	2122.0
94.10	4478.0
95.10	36856.0
96.10	2624.0
103.90	148.0
105.80	162.0
115.90	115.0
117.00	400.0
117.90	155.0
119.10	353.0
128.00	214.0
135.00	139.0
137.00	118.0
141.00	582.0
143.00	855.0
143.90	136.0
144.80	312.0
145.90	140.0
154.80	153.0
171.90	751.0
172.60	424.0
173.20	469.0
174.00	35904.0
175.00	2380.0
176.00	35736.0
177.00	2543.0

Instrument :
MSVOA_V
ClientSampleId :
BFB832

m/z	Abundance
39.90	241.0

Instrument :
MSVOA_V
ClientSampleId :
BFB832

m/z	Abundance
35.10	114.0
36.00	218.0
37.00	1021.0
38.00	1084.0
39.10	521.0
39.90	183.0
43.90	503.0
45.20	247.0
47.20	198.0
48.10	210.0
49.00	1340.0
50.10	5758.0
51.10	1605.0
52.10	138.0
56.10	596.0
57.00	1215.0
60.10	444.0
61.20	1570.0
62.00	1509.0
63.00	1277.0
64.10	213.0
65.10	397.0
68.00	2824.0
69.00	3932.0
70.00	155.0
72.10	198.0
73.00	1215.0
74.10	5818.0
75.00	17784.0
76.00	1592.0
77.00	204.0
77.40	140.0
79.00	1071.0
79.80	243.0
81.00	1086.0
81.90	272.0
86.90	1270.0
88.00	1326.0
91.10	101.0
92.00	1296.0
93.10	2011.0
94.10	4185.0
95.10	33624.0
96.00	2489.0
103.90	128.0
105.90	190.0
117.00	289.0
117.90	113.0
119.00	313.0
127.90	197.0
137.00	143.0
140.90	540.0
143.00	706.0
143.90	118.0
144.80	275.0
145.90	153.0
154.80	175.0
159.10	122.0
171.90	572.0
172.60	464.0
174.00	33168.0
175.00	2181.0
176.00	31152.0
177.00	2417.0

Instrument :
MSVOA_V
ClientSampleId :
BFB832