

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041619\
 Data File : VV010339.D
 Acq On : 16 Apr 2019 18:09
 Operator : SY/MD
 Sample : K2402-17
 Misc : 5.08G/10mL/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAHJ7

Quant Time: Apr 16 23:48:40 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041019S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 16 23:09:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	318069	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	312043	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	155002	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	50741	13.86	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	55.44%
7) Chloroethane-d5	1.57	69	56960	18.10	ug/L	0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.40%
10) 1,1-Dichloroethene-d2	2.13	63	114189	12.25	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.00%
20) 2-Butanone-d5	3.93	46	53111	57.32	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.64%
24) Chloroform-d	4.40	84	148742	20.48	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.92%
26) 1,2-Dichloroethane-d4	5.08	65	95280	23.03	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.12%
29) Benzene-d6	5.10	84	289284	19.23	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	76.92%
33) 1,2-Dichloropropane-d6	6.12	67	92238	20.61	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.44%
37) Toluene-d8	7.36	98	265059	18.06	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.24%
38) trans-1,3-Dichloropropene-	7.66	79	36212	19.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.64%
39) 2-Hexanone-d5	8.13	63	35401	45.80	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.60%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	96311	23.98	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.92%
61) 1,2-Dichlorobenzene-d4	11.67	152	126900	22.17	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.68%


Target Compounds					Ovalue
13) Acetone	2.18	43	4991	5.041 ug/L	93
15) Methyl Acetate	2.46	43	2416	1.370 ug/L	96
16) Methylene chloride	2.54	84	20630	3.312 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV041619\
Data File : VV010339.D
Acq On : 16 Apr 2019 18:09
Operator : SY/MD
Sample : K2402-17
Misc : 5.08G/10mL/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAHJ7

Quant Time: Apr 16 23:48:40 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041019S.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 16 23:09:02 2019
Response via : Initial Calibration

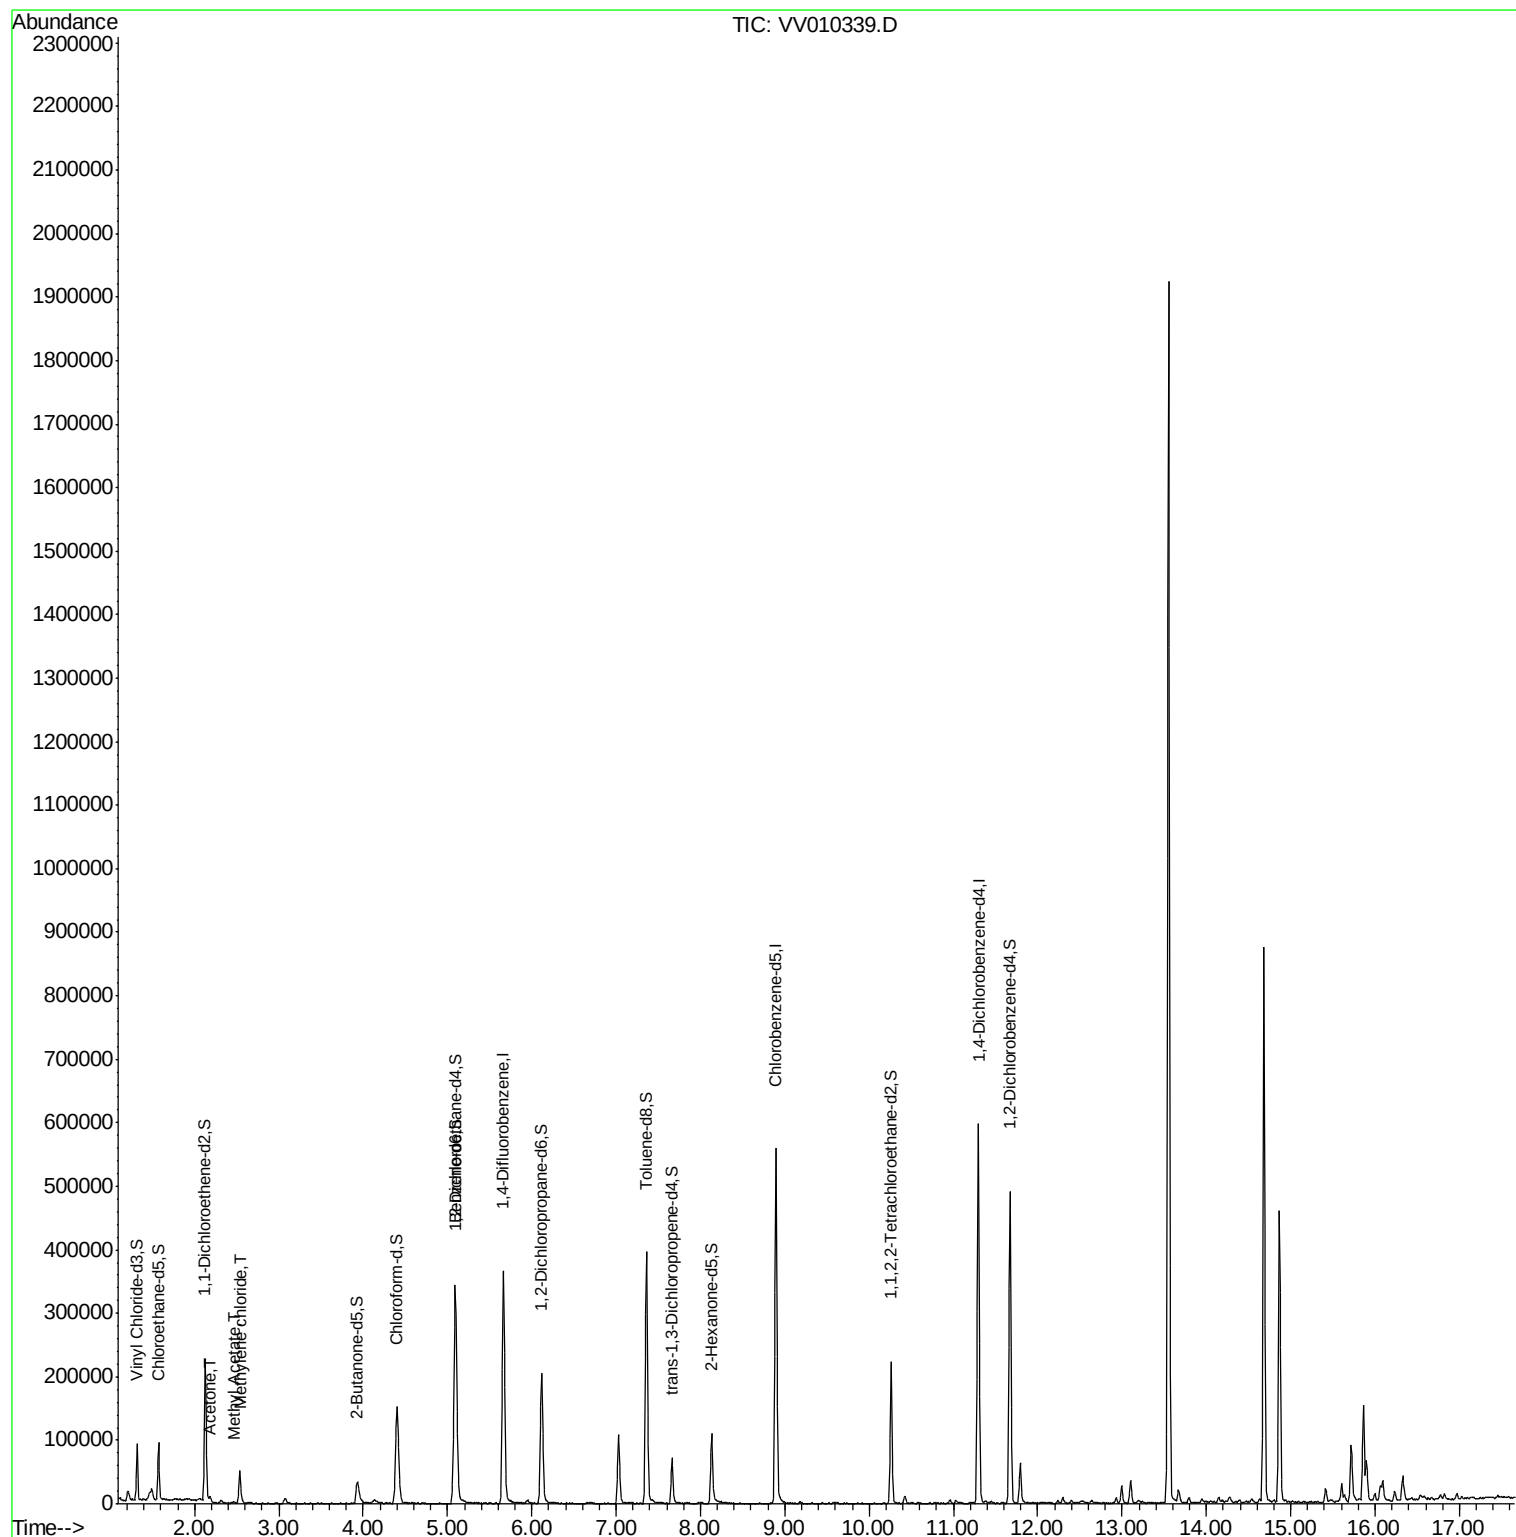

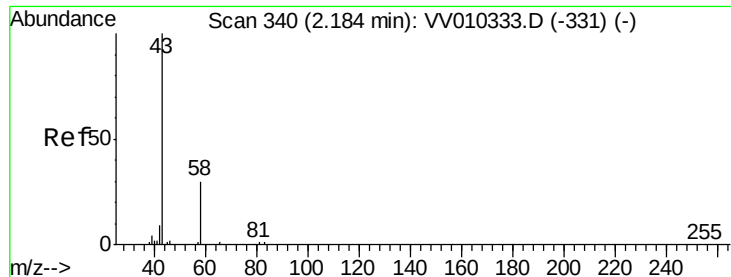

#13

Acetone

Concen: 5.041 ug/L

RT: 2.18 min Scan# 340

Delta R.T. -0.00 min

Lab File: VV010339.D

Acq: 16 Apr 2019 18:09

Instrument :

MSVOA_V

ClientSampleId :





GAHJ7

Tot Ion: 43 Resp: 4991

Ion Ratio Lower Upper

43 100

58 34.6 0.0 61.6

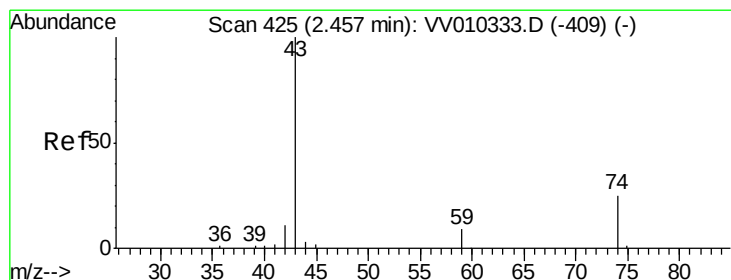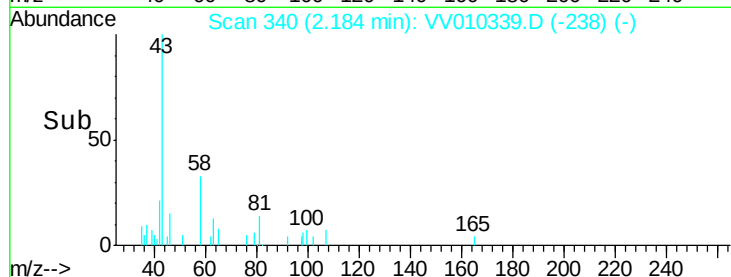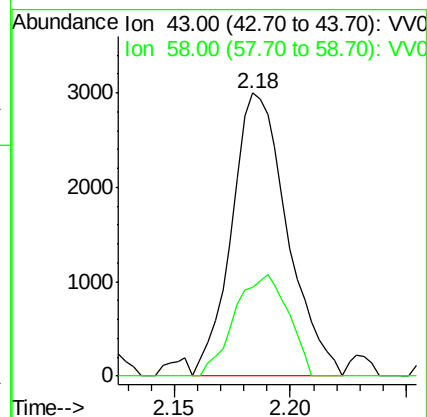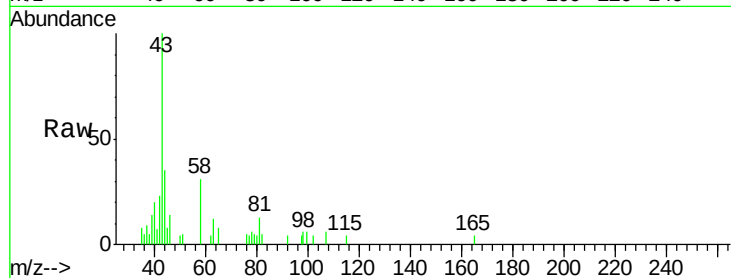

#15

Methyl Acetate

Concen: 1.370 ug/L

RT: 2.46 min Scan# 427

Delta R.T. 0.01 min

Lab File: VV010339.D




Acq: 16 Apr 2019 18:09




Tgt Ion: 43 Resp: 2416

Ion Ratio Lower Upper

43 100

74 25.9 19.3 28.9

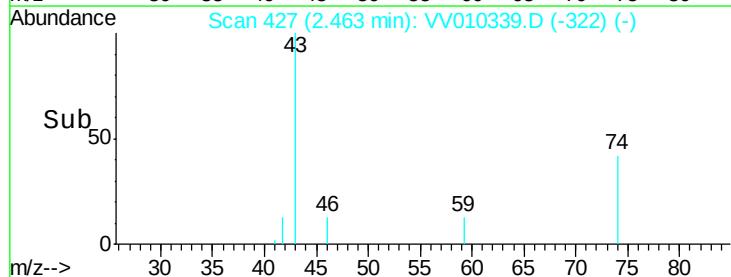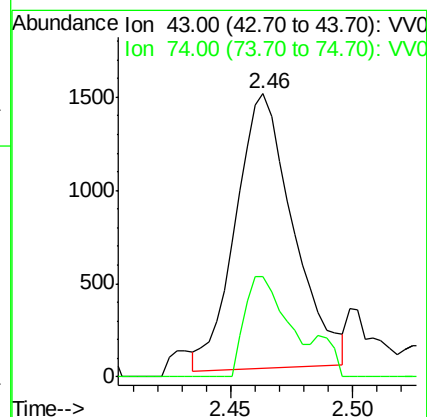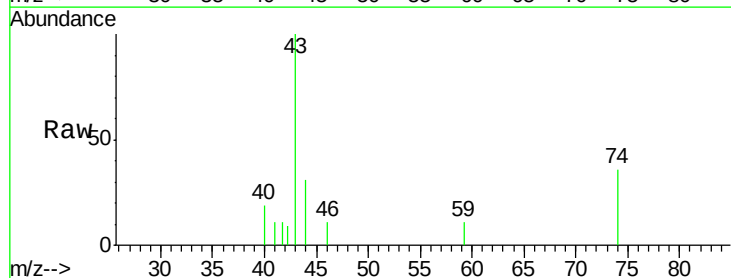

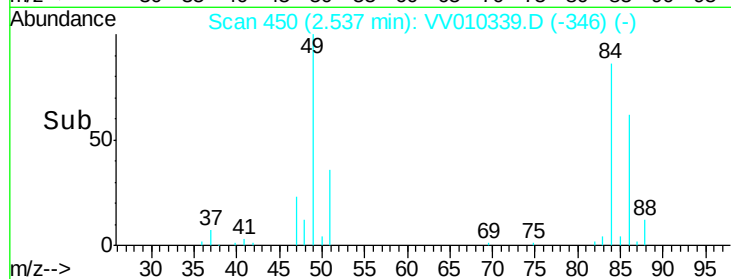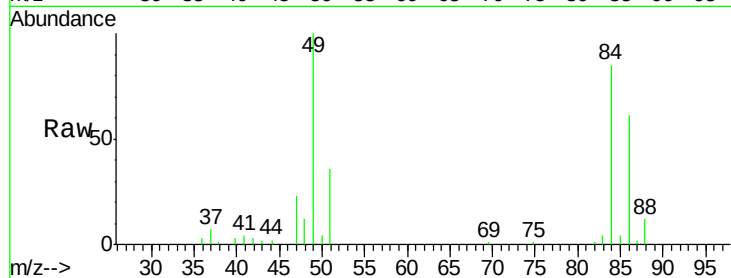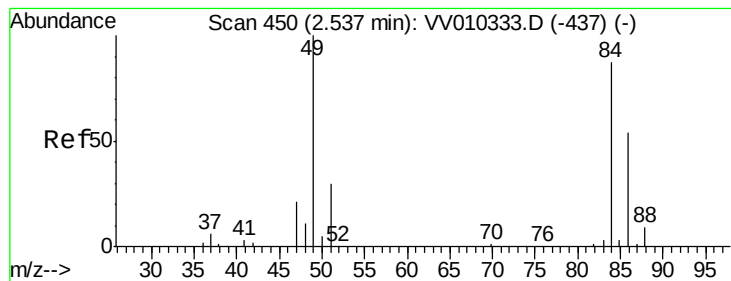

#16

Methylene chloride

Concen: 3.312 ug/L

RT: 2.54 min Scan# 450

Delta R.T. 0.00 min

Lab File: VV010339.D

Acq: 16 Apr 2019 18:09

Instrument :

MSVOA_V

ClientSampleId :

GAHJ7

Tot Ion: 84 Resp: 20630

Ion Ratio Lower Upper

84 100

49 117.9 79.9 148.5

86 71.9 44.5 82.7

