

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041620\
 Data File : VV015537.D
 Acq On : 16 Apr 2020 15:24
 Operator : SY/MD
 Sample : L2320-04
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFRR1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.139	8	15	25	rVB2	64729	70829	5.29%	1.106%
2	1.312	62	69	78	rVB	44089	44957	3.36%	0.702%
3	1.576	143	151	167	rVB	40176	47248	3.53%	0.738%
4	1.759	199	208	225	rVB	519093	690833	51.62%	10.786%
5	2.119	310	320	339	rVB3	96277	159731	11.94%	2.494%
6	2.785	514	527	548	rBV2	50976	121310	9.06%	1.894%
7	3.212	646	660	675	rBV2	14054	29836	2.23%	0.466%
8	3.942	872	887	952	rBV4	57946	256891	19.20%	4.011%
9	4.376	1005	1022	1047	rBV	56093	150133	11.22%	2.344%
10	5.071	1221	1238	1268	rBV2	129173	320209	23.93%	5.000%
11	5.640	1402	1415	1443	rBV	129764	260075	19.43%	4.061%
12	5.936	1493	1507	1538	rBV	527681	1022981	76.44%	15.972%
13	6.097	1544	1557	1581	rVB	76085	156302	11.68%	2.440%
14	7.010	1830	1841	1864	rBV	40265	74141	5.54%	1.158%
15	7.338	1930	1943	1961	rBV	154314	270736	20.23%	4.227%
16	7.646	2029	2039	2061	rBV	23880	42138	3.15%	0.658%
17	7.997	2127	2148	2175	rBV	787826	1338285	100.00%	20.896%
18	8.116	2175	2185	2226	rVB	182445	354683	26.50%	5.538%
19	8.875	2407	2421	2444	rBV	196231	320087	23.92%	4.998%
20	10.238	2835	2845	2862	rVB	52486	80296	6.00%	1.254%
21	11.270	3155	3166	3190	rBV	208141	335193	25.05%	5.234%
22	11.646	3272	3283	3303	rBV	159417	257755	19.26%	4.024%


Sum of corrected areas: 6404649

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV041620\
Data File : VV015537.D
Acq On : 16 Apr 2020 15:24
Operator : SY/MD
Sample : L2320-04
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFRR1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

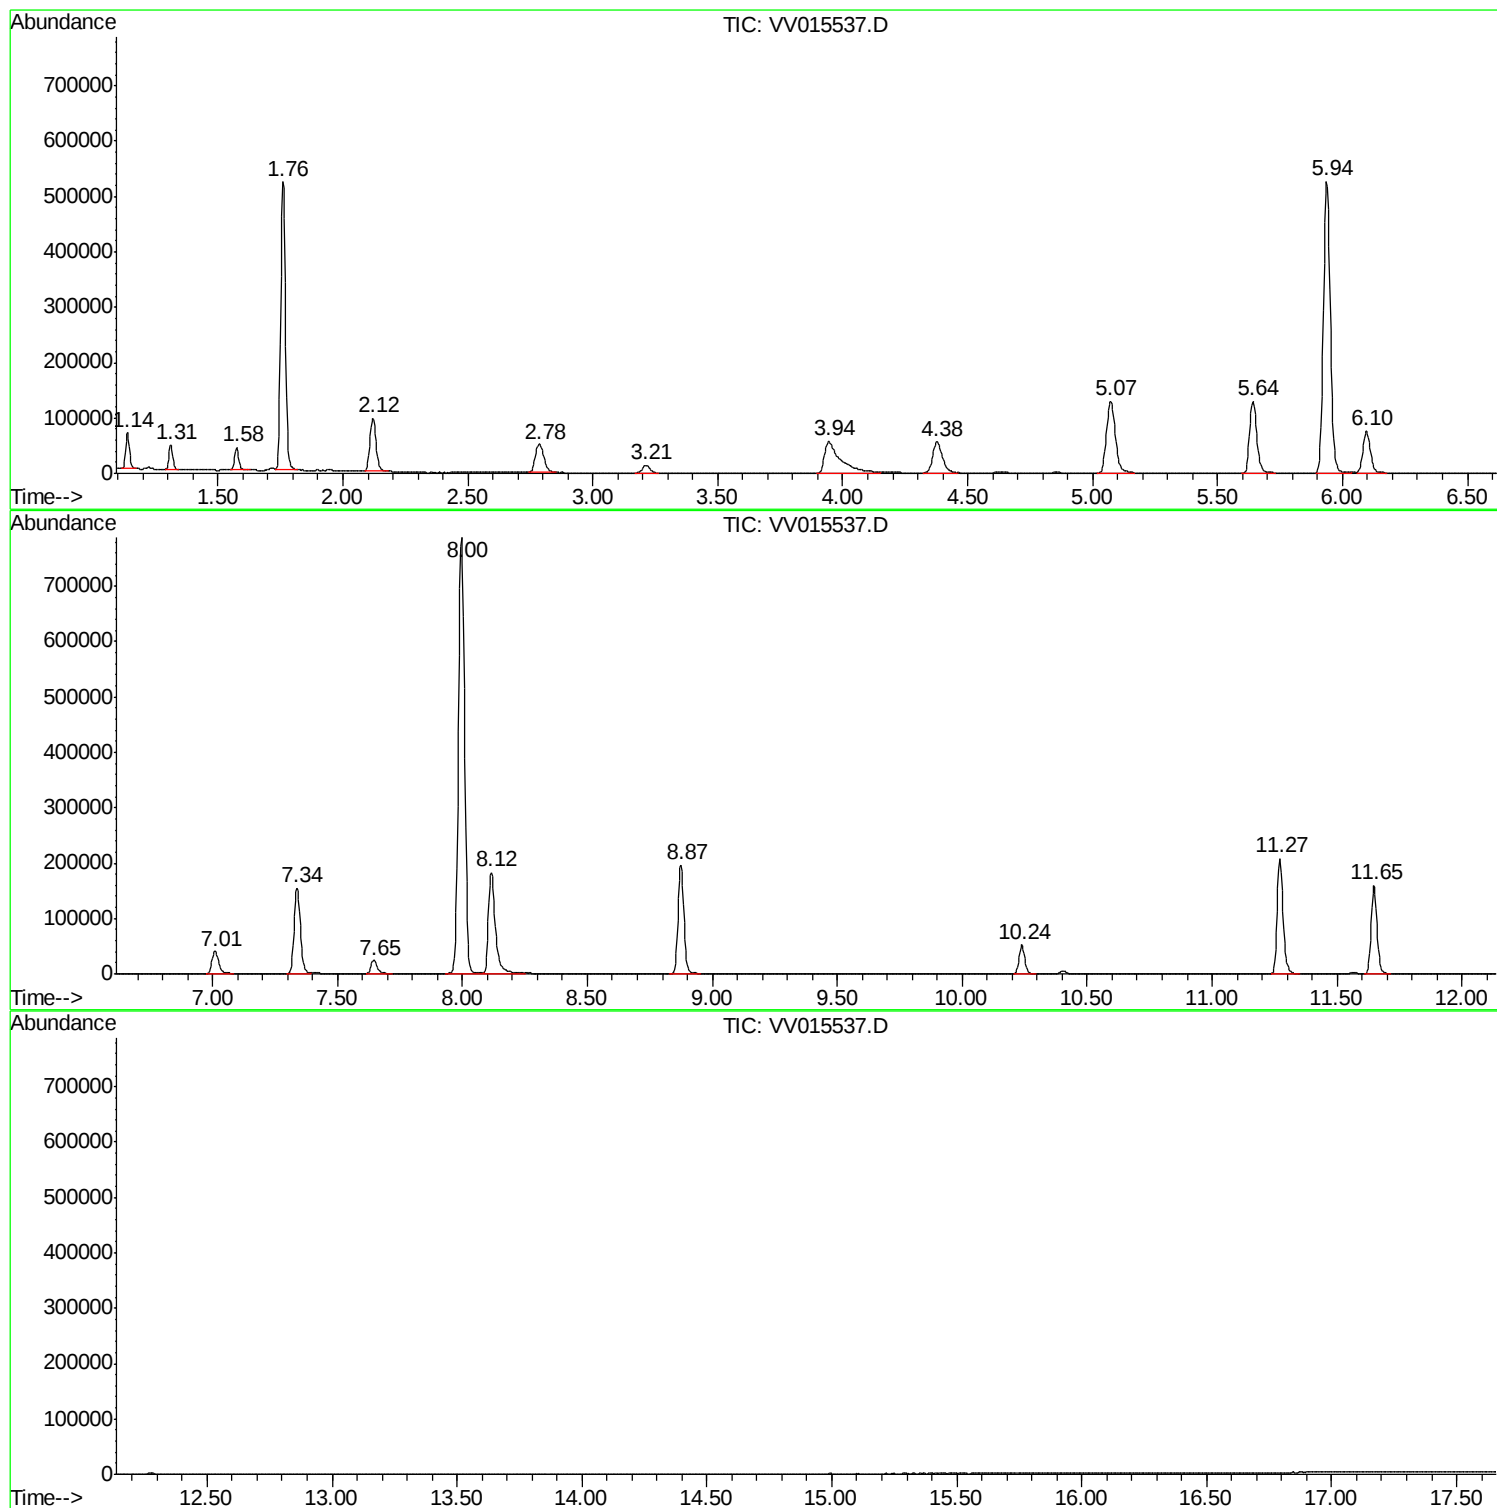

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV041620\
Data File : VV015537.D
Acq On : 16 Apr 2020 15:24
Operator : SY/MD
Sample : L2320-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFRR1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV041620\
Data File : VV015537.D
Acq On : 16 Apr 2020 15:24
Operator : SY/MD
Sample : L2320-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFRR1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc