


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV041620\
 Data File : VV015525.D
 Acq On : 16 Apr 2020 09:43
 Operator : SY/MD
 Sample : BFB36
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB36

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Apr 17 00:46:36 2020

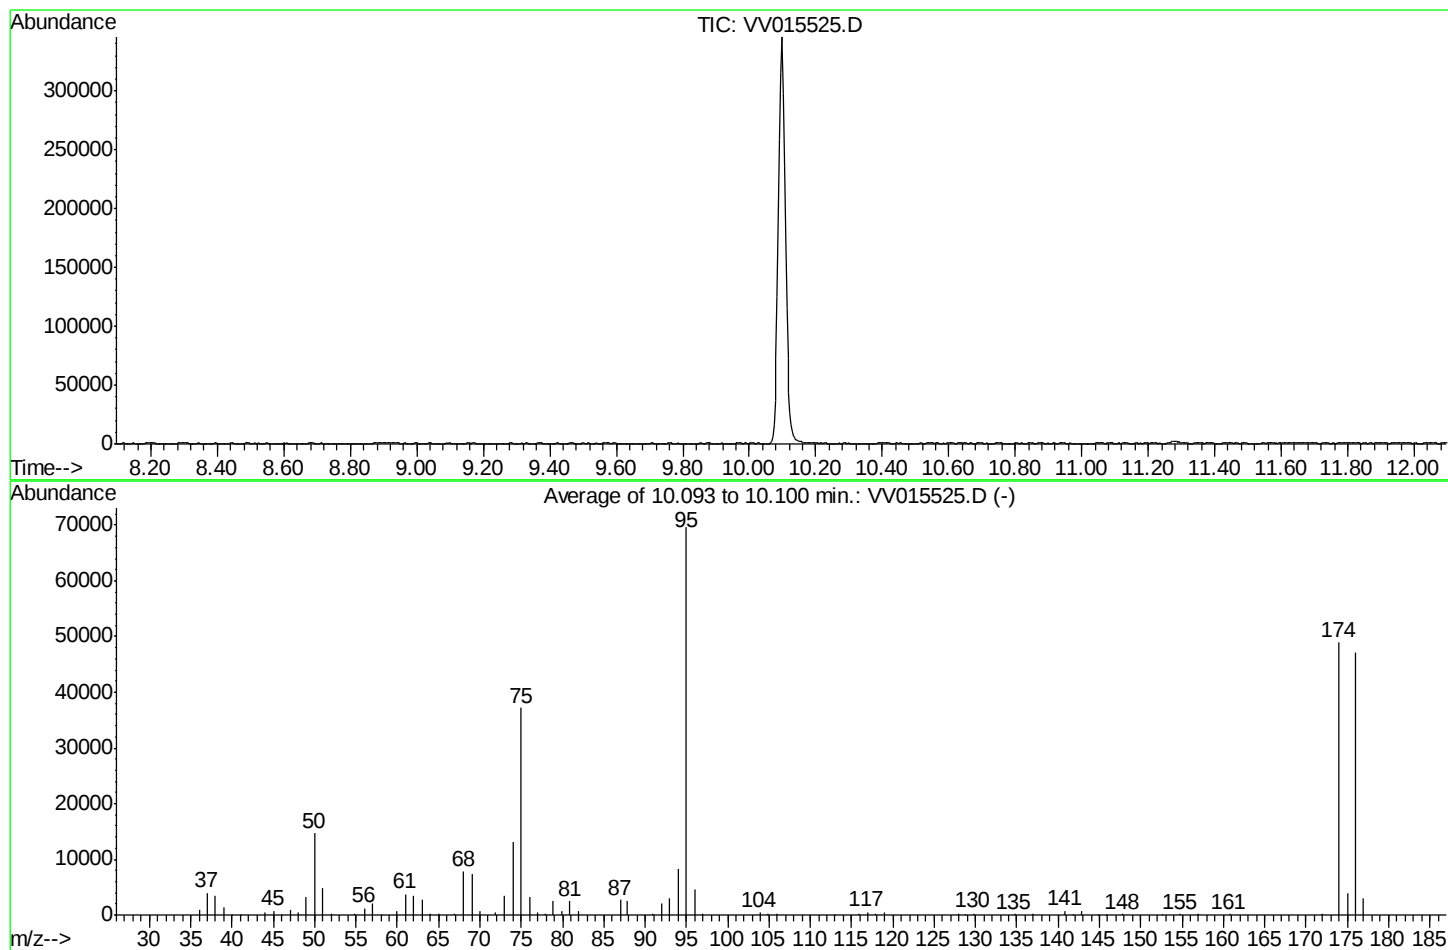

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	14676	PASS
75	95	30	80	53.4	37168	PASS
95	95	100	100	100.0	69610	PASS
96	95	5	9	6.7	4676	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.2	48850	PASS
175	174	5	9	7.9	3856	PASS
176	174	95	101	96.6	47192	PASS
177	176	5	9	6.4	2998	PASS

m/z	Abundance
36.00	799.0
37.00	3755.0
38.00	3550.0
39.00	1412.0
39.90	294.0
43.90	734.0
45.00	680.0
46.00	113.0
47.00	901.0
47.90	453.0
49.00	3327.0
50.00	14083.0
51.00	4670.0
52.00	220.0
54.90	181.0
56.00	1123.0
57.00	1979.0
58.00	118.0
60.00	703.0
61.00	3653.0
62.00	3379.0
63.00	2500.0
64.00	307.0
65.10	216.0
66.90	221.0
68.00	7602.0
69.00	7070.0
70.00	668.0
71.90	395.0
73.00	3245.0
74.00	12734.0
75.00	35448.0
76.00	3034.0
77.00	486.0
77.90	253.0
78.90	2418.0
79.90	650.0
80.90	2381.0
81.90	643.0
87.00	2568.0
87.90	2382.0
90.90	314.0
92.00	1937.0
93.00	2952.0
94.00	7755.0
95.00	65880.0
96.00	4530.0
97.00	151.0
103.90	371.0
104.70	134.0
105.90	323.0
115.80	312.0
116.90	445.0
117.90	322.0
118.90	360.0
127.90	225.0
128.80	114.0
129.80	246.0
134.80	159.0
136.90	178.0
140.90	737.0
141.80	115.0
142.80	727.0
144.90	101.0
147.80	147.0
154.80	154.0
156.90	135.0
160.80	134.0
172.00	246.0
174.00	44968.0
175.00	3526.0
176.00	43480.0
177.00	2760.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
36.00	882.0
37.00	4060.0
38.00	3665.0
39.00	1412.0
39.90	288.0
43.90	729.0
45.00	747.0
46.00	114.0
47.00	943.0
47.90	492.0
49.00	3429.0
50.00	15119.0
51.00	4948.0
52.00	213.0
54.90	178.0
56.00	1215.0
57.00	2171.0
58.00	108.0
60.00	823.0
61.00	3891.0
62.00	3647.0
63.00	2843.0
64.00	336.0
65.10	213.0
66.90	223.0
68.00	8060.0
69.00	7717.0
70.00	630.0
71.90	436.0
73.00	3439.0
74.00	13605.0
75.00	38528.0
76.00	3276.0
77.00	491.0
77.90	289.0
78.90	2585.0
79.90	715.0
80.90	2566.0
81.90	675.0
87.00	2905.0
87.90	2609.0
90.90	328.0
92.00	2196.0
93.00	3015.0
94.00	8564.0
95.00	72344.0
96.00	4832.0
97.00	156.0
103.90	410.0
104.80	136.0
105.90	340.0
115.80	317.0
116.90	522.0
117.80	335.0
118.90	429.0
127.90	242.0
128.80	129.0
129.80	259.0
134.80	193.0
136.90	184.0
140.80	819.0
141.80	118.0
142.90	784.0
144.90	118.0
145.80	115.0
147.80	169.0
152.60	105.0
154.80	162.0
156.90	150.0
160.80	132.0
172.00	272.0
174.00	50672.0
175.00	3997.0
176.00	48984.0
177.00	3101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
36.00	893.0
37.00	4045.0
38.00	3388.0
39.00	1312.0
39.90	282.0
41.00	109.0
43.90	671.0
45.00	692.0
47.00	861.0
48.00	474.0
49.00	3199.0
50.00	14828.0
51.00	4688.0
52.00	181.0
54.80	162.0
56.00	1169.0
57.00	2138.0
59.90	808.0
61.00	3714.0
62.00	3519.0
63.00	2886.0
64.00	275.0
65.00	208.0
66.90	218.0
68.00	7581.0
69.00	7587.0
70.00	569.0
71.90	430.0
73.00	3423.0
74.00	12948.0
75.00	37528.0
76.00	3192.0
77.00	422.0
77.90	303.0
78.90	2590.0
79.90	735.0
80.90	2455.0
81.90	624.0
87.00	2802.0
87.90	2579.0
90.80	331.0
92.00	2162.0
93.00	2814.0
94.00	8386.0
95.00	70608.0
96.00	4666.0
97.00	153.0
103.90	432.0
104.90	132.0
105.90	337.0
112.90	106.0
115.80	287.0
116.90	540.0
117.80	298.0
118.90	451.0
127.90	264.0
128.80	110.0
129.80	253.0
134.70	178.0
136.90	162.0
140.80	794.0
141.80	110.0
142.90	824.0
144.80	116.0
145.80	131.0
147.90	184.0
154.80	169.0
156.90	138.0
160.80	109.0
171.90	265.0
174.00	50912.0
175.00	4046.0
176.00	49112.0
177.00	3134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

Scan 2788 (10.055 min): VV015525.D
BFB36

m/z	Abundance
39.90	281.0
43.90	280.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36