

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021038.D
 Acq On : 16 Apr 2021 10:25
 Operator : SY/MD
 Sample : VV0416WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK165

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

Signal : TIC: VV021038.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	101	rVB	182121	195488	11.64%	1.493%
2	1.571	158	165	183	rVB	148347	187221	11.15%	1.430%
3	2.108	323	332	345	rBV	393696	562252	33.47%	4.293%
4	2.297	383	391	397	rVB5	2432	3574	0.21%	0.027%
5	2.510	452	457	471	rVB6	3846	6415	0.38%	0.049%
6	2.703	515	517	521	rVB2	485	268	0.02%	0.002%
7	2.728	521	525	527	rBV	336	286	0.02%	0.002%
8	2.760	533	535	538	rBV3	797	616	0.04%	0.005%
9	2.876	569	571	575	rVB2	471	353	0.02%	0.003%
10	2.902	576	579	581	rBV2	423	346	0.02%	0.003%
11	3.535	773	776	779	rBV2	504	268	0.02%	0.002%
12	3.789	852	855	859	rVB2	361	293	0.02%	0.002%
13	3.844	868	872	879	rVB2	434	448	0.03%	0.003%
14	3.912	882	893	937	rBV	66507	284000	16.91%	2.169%
15	4.352	1016	1030	1057	rVB2	292784	729125	43.40%	5.568%
16	4.577	1097	1100	1104	rVB2	728	554	0.03%	0.004%
17	4.603	1104	1108	1109	rBV2	690	407	0.02%	0.003%
18	4.651	1121	1123	1128	rBV2	447	338	0.02%	0.003%
19	4.876	1191	1193	1197	rVB	594	360	0.02%	0.003%
20	4.928	1207	1209	1212	rBV	452	304	0.02%	0.002%
21	5.050	1231	1247	1278	rBV2	652569	1679853	100.00%	12.828%
22	5.252	1307	1310	1311	rBV	573	285	0.02%	0.002%
23	5.297	1322	1324	1329	rBV2	552	330	0.02%	0.003%
24	5.452	1369	1372	1376	rVB2	429	288	0.02%	0.002%
25	5.474	1376	1379	1381	rBV2	568	340	0.02%	0.003%
26	5.532	1395	1397	1400	rBV2	579	333	0.02%	0.003%
27	5.619	1412	1424	1451	rBV	540455	1079915	64.29%	8.246%
28	5.805	1480	1482	1484	rBV2	518	261	0.02%	0.002%
29	5.873	1500	1503	1506	rBV3	767	517	0.03%	0.004%
30	5.905	1510	1513	1514	rBV3	1033	596	0.04%	0.005%
31	5.998	1539	1542	1545	rBV2	447	338	0.02%	0.003%
32	6.072	1550	1565	1587	rBV	359899	737711	43.92%	5.633%
33	6.217	1607	1610	1618	rBV5	1106	1251	0.07%	0.010%
34	6.310	1637	1639	1642	rBV	462	275	0.02%	0.002%
35	6.326	1642	1644	1647	rVV3	967	492	0.03%	0.004%
36	6.420	1669	1673	1681	rVV3	587	814	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021038.D
 Acq On : 16 Apr 2021 10:25
 Operator : SY/MD
 Sample : VV0416WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK165

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.567	1717	1719	1725	rVB2	581	541	0.03%	0.004%
38	6.600	1725	1729	1731	rBV2	525	484	0.03%	0.004%
39	6.747	1767	1775	1777	rBV	613	513	0.03%	0.004%
40	6.889	1817	1819	1824	rBV2	412	338	0.02%	0.003%
41	6.921	1827	1829	1833	rVB2	703	422	0.03%	0.003%
42	6.989	1838	1850	1873	rBV	214218	393002	23.40%	3.001%
43	7.217	1918	1921	1923	rBV	585	436	0.03%	0.003%
44	7.320	1941	1953	1971	rBV	797229	1383633	82.37%	10.566%
45	7.625	2038	2048	2070	rBV2	154351	271672	16.17%	2.075%
46	7.857	2118	2120	2122	rVB3	859	346	0.02%	0.003%
47	7.895	2128	2132	2133	rBV	500	386	0.02%	0.003%
48	7.937	2140	2145	2146	rBV4	692	567	0.03%	0.004%
49	8.018	2166	2170	2172	rBV	880	555	0.03%	0.004%
50	8.095	2179	2194	2218	rBV	379806	688891	41.01%	5.261%
51	8.336	2267	2269	2271	rBV2	642	340	0.02%	0.003%
52	8.503	2319	2321	2324	rBV	507	378	0.02%	0.003%
53	8.580	2342	2345	2347	rBV	483	323	0.02%	0.002%
54	8.690	2373	2379	2382	rBV4	484	488	0.03%	0.004%
55	8.747	2395	2397	2403	rBV	387	413	0.02%	0.003%
56	8.773	2403	2405	2411	rVB2	407	295	0.02%	0.002%
57	8.805	2411	2415	2416	rBV	432	328	0.02%	0.003%
58	8.857	2419	2431	2454	rBV	812844	1308192	77.88%	9.990%
59	9.069	2494	2497	2500	rBV3	564	401	0.02%	0.003%
60	9.207	2538	2540	2543	rBV2	434	296	0.02%	0.002%
61	9.288	2559	2565	2567	rBV2	403	387	0.02%	0.003%
62	9.477	2619	2624	2626	rBV2	472	368	0.02%	0.003%
63	9.506	2629	2633	2638	rVB3	506	546	0.03%	0.004%
64	9.535	2638	2642	2643	rBV3	602	350	0.02%	0.003%
65	9.715	2695	2698	2701	rVB2	643	408	0.02%	0.003%
66	9.738	2701	2705	2706	rBV2	330	263	0.02%	0.002%
67	9.940	2763	2768	2770	rBV2	876	611	0.04%	0.005%
68	10.133	2822	2828	2838	rVB4	2943	4119	0.25%	0.031%
69	10.220	2840	2855	2876	rBV	572024	904178	53.82%	6.905%
70	10.542	2951	2955	2956	rBV	1144	673	0.04%	0.005%
71	10.596	2970	2972	2975	rBV2	762	419	0.02%	0.003%
72	10.728	3011	3013	3017	rBV	572	448	0.03%	0.003%
73	10.815	3035	3040	3045	rBV2	556	587	0.03%	0.004%
74	10.905	3063	3068	3069	rBV3	886	619	0.04%	0.005%
75	10.924	3070	3074	3082	rVB5	4025	4846	0.29%	0.037%
76	11.123	3133	3136	3138	rVB	611	375	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021038.D
 Acq On : 16 Apr 2021 10:25
 Operator : SY/MD
 Sample : VV0416WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK165

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	11.149	3138	3144	3148	rBV4	1360	1482	0.09%	0.011%
78	11.255	3166	3177	3202	rBV	785412	1229263	73.18%	9.387%
79	11.390	3217	3219	3220	rBV	1206	536	0.03%	0.004%
80	11.477	3242	3246	3251	rBV	798	677	0.04%	0.005%
81	11.632	3281	3294	3315	rBV	902476	1389098	82.69%	10.607%
82	11.789	3339	3343	3345	rBV	586	572	0.03%	0.004%
83	11.895	3374	3376	3379	rBV	742	455	0.03%	0.003%
84	12.008	3409	3411	3416	rVB	458	288	0.02%	0.002%
85	12.213	3471	3475	3476	rBV	485	275	0.02%	0.002%
86	12.419	3536	3539	3542	rBV2	395	311	0.02%	0.002%
87	12.435	3542	3544	3549	rVB2	715	373	0.02%	0.003%
88	12.541	3575	3577	3582	rBV2	547	320	0.02%	0.002%
89	12.567	3582	3585	3587	rBV	576	266	0.02%	0.002%
90	12.660	3606	3614	3623	rVB7	3188	5216	0.31%	0.040%
91	12.866	3675	3678	3683	rBV2	483	352	0.02%	0.003%
92	13.098	3744	3750	3752	rBV	504	543	0.03%	0.004%
93	13.239	3791	3794	3797	rBV2	635	444	0.03%	0.003%
94	13.278	3800	3806	3817	rVB4	4881	6482	0.39%	0.049%
95	13.377	3834	3837	3841	rVV3	590	460	0.03%	0.004%
96	13.406	3842	3846	3849	rBV	680	522	0.03%	0.004%
97	13.654	3920	3923	3926	rBV3	514	391	0.02%	0.003%
98	13.757	3950	3955	3967	rVB7	4872	7117	0.42%	0.054%
99	13.914	4002	4004	4006	rBV	892	413	0.02%	0.003%
100	14.561	4202	4205	4209	rVB	868	677	0.04%	0.005%




Sum of corrected areas: 13095485

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021038.D
Acq On : 16 Apr 2021 10:25
Operator : SY/MD
Sample : VV0416WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK165

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

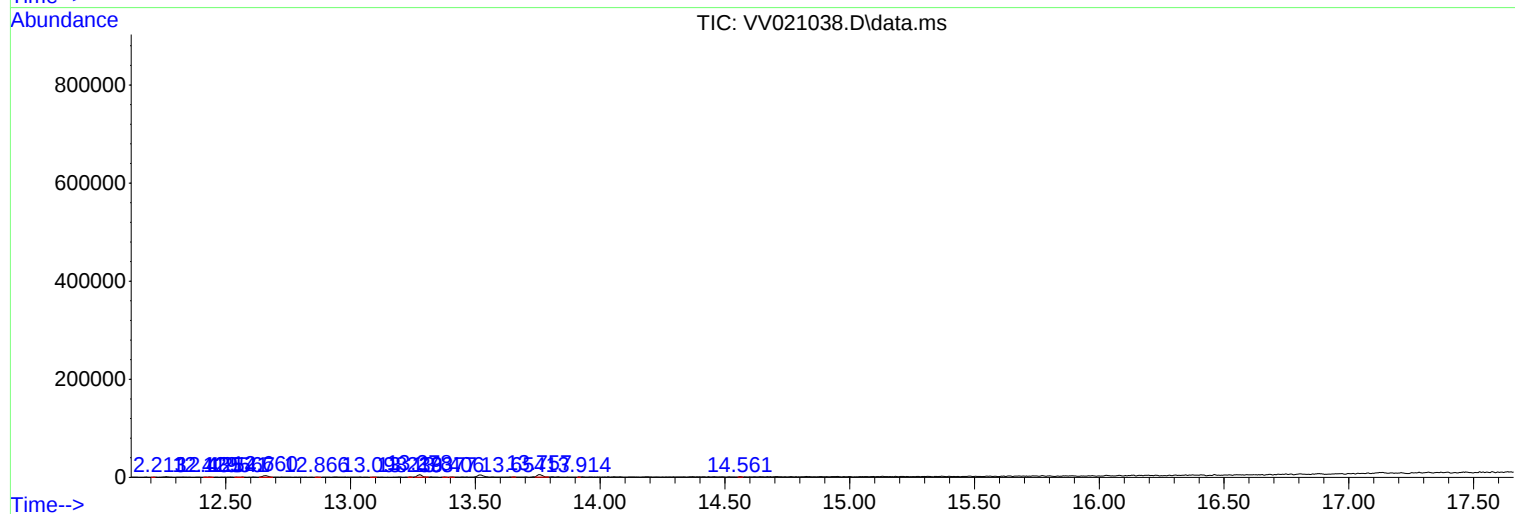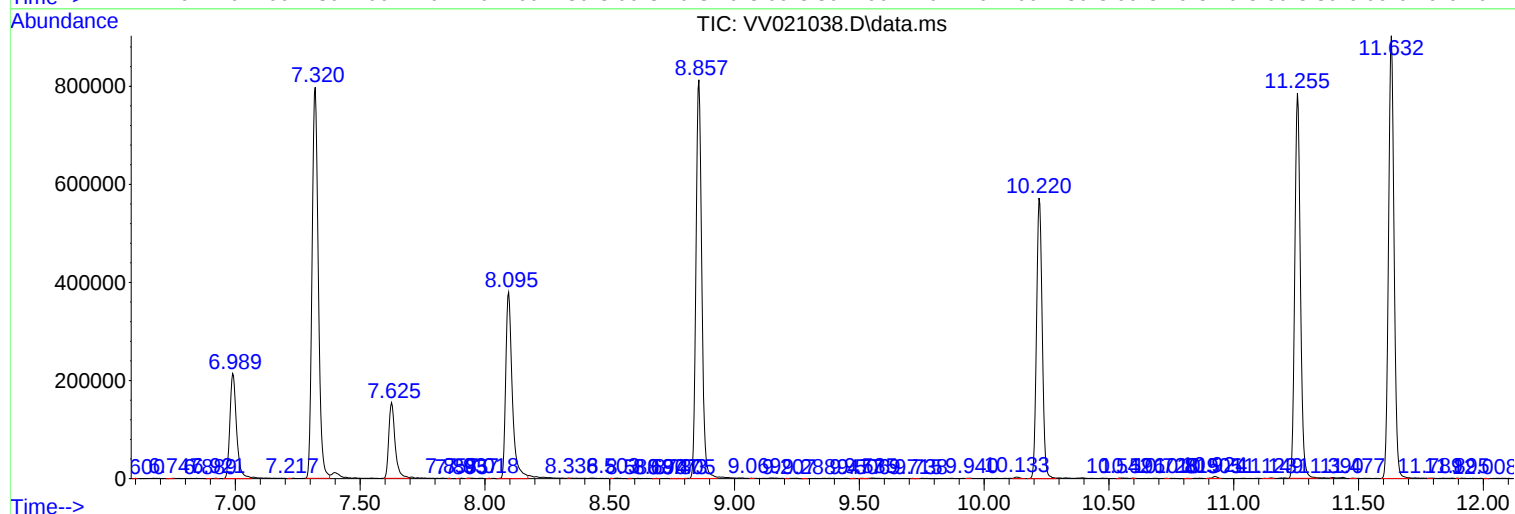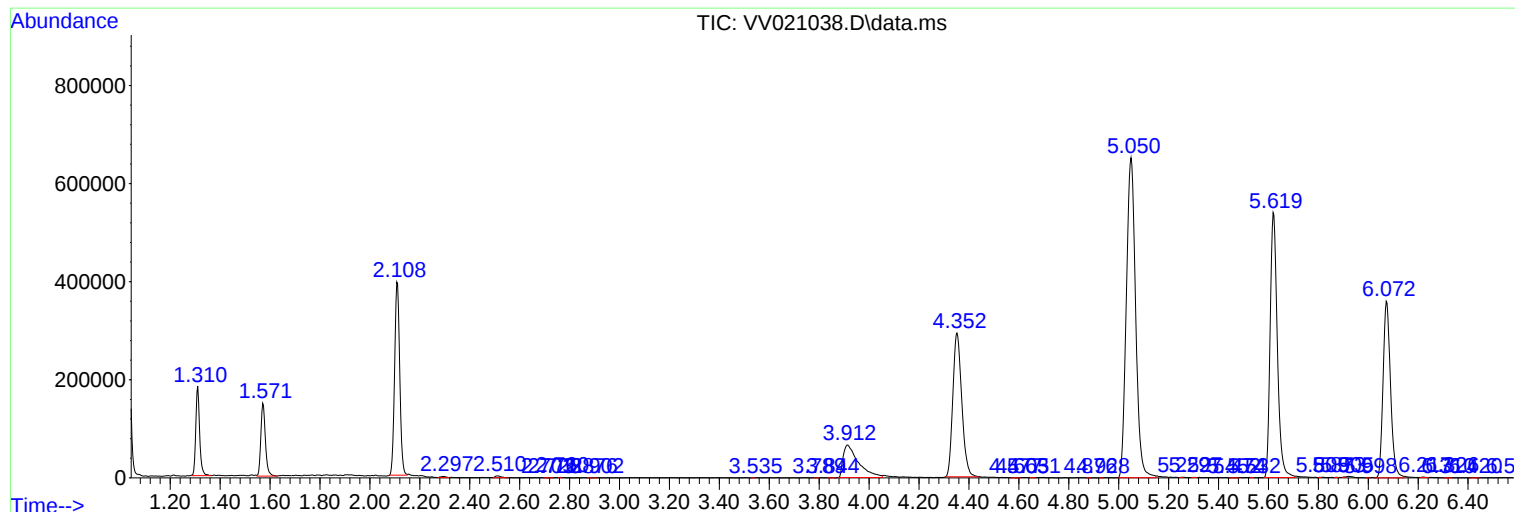

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021038.D
Acq On : 16 Apr 2021 10:25
Operator : SY/MD
Sample : VV0416WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK165

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021038.D
Acq On : 16 Apr 2021 10:25
Operator : SY/MD
Sample : VV0416WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK165

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
