

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021039.D
 Acq On : 16 Apr 2021 11:41
 Operator : SY/MD
 Sample : M2031-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG541

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M

Title : VOC Analysis

Signal : TIC: VV021039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	78	84	103	rVB	165948	180718	11.00%	1.353%
2	1.571	158	165	182	rVB	139971	179768	10.95%	1.346%
3	2.111	323	333	349	rBV	364360	529895	32.27%	3.967%
4	2.423	428	430	434	rBV3	652	442	0.03%	0.003%
5	2.452	434	439	442	rBV4	1101	1139	0.07%	0.009%
6	2.510	453	457	460	rBV3	1058	988	0.06%	0.007%
7	2.587	476	481	484	rBV2	883	885	0.05%	0.007%
8	2.622	487	492	495	rBV4	673	783	0.05%	0.006%
9	2.844	559	561	564	rBV	457	297	0.02%	0.002%
10	3.108	637	643	647	rBB	564	577	0.04%	0.004%
11	3.195	664	670	672	rBV3	519	482	0.03%	0.004%
12	3.243	683	685	690	rBV	402	365	0.02%	0.003%
13	3.285	695	698	702	rBV2	393	391	0.02%	0.003%
14	3.442	746	747	751	rVB	447	282	0.02%	0.002%
15	3.471	752	756	759	rBV2	419	292	0.02%	0.002%
16	3.510	764	768	772	rVB2	341	295	0.02%	0.002%
17	3.690	819	824	828	rBV2	480	550	0.03%	0.004%
18	3.722	829	834	835	rBV3	900	577	0.04%	0.004%
19	3.841	867	871	875	rBV3	549	497	0.03%	0.004%
20	3.902	878	890	919	rBV	68258	250003	15.22%	1.872%
21	4.252	996	999	1000	rBV	662	375	0.02%	0.003%
22	4.349	1012	1029	1064	rBV	289492	733464	44.66%	5.491%
23	4.522	1076	1083	1089	rBV5	786	1121	0.07%	0.008%
24	4.709	1137	1141	1144	rBV3	530	387	0.02%	0.003%
25	4.805	1166	1171	1173	rBV2	738	596	0.04%	0.004%
26	4.828	1173	1178	1180	rBV3	660	593	0.04%	0.004%
27	5.047	1229	1246	1278	rBV2	627128	1642178	100.00%	12.295%
28	5.262	1309	1313	1314	rBV2	659	473	0.03%	0.004%
29	5.545	1396	1401	1402	rBV	502	366	0.02%	0.003%
30	5.619	1411	1424	1455	rVV	598655	1197143	72.90%	8.963%
31	5.818	1483	1486	1490	rVB3	791	546	0.03%	0.004%
32	5.921	1507	1518	1525	rVV6	2156	3886	0.24%	0.029%
33	5.953	1526	1528	1532	rVB3	625	387	0.02%	0.003%
34	6.072	1550	1565	1593	rBV	348724	717139	43.67%	5.369%
35	6.368	1653	1657	1661	rVB5	809	576	0.04%	0.004%
36	6.474	1687	1690	1695	rVB2	686	554	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021039.D
 Acq On : 16 Apr 2021 11:41
 Operator : SY/MD
 Sample : M2031-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG541

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

37	6.503	1696	1699	1702	rBV	673	422	0.03%	0.003%
38	6.526	1703	1706	1708	rVV	1065	608	0.04%	0.005%
39	6.538	1708	1710	1717	rVB4	597	521	0.03%	0.004%
40	6.654	1741	1746	1747	rBV2	689	478	0.03%	0.004%
41	6.793	1787	1789	1793	rVB	524	286	0.02%	0.002%
42	6.902	1817	1823	1824	rBV	329	318	0.02%	0.002%
43	6.937	1829	1834	1838	rBV2	1022	1174	0.07%	0.009%
44	6.985	1839	1849	1874	rBV	207606	384337	23.40%	2.878%
45	7.182	1905	1910	1912	rBV2	726	619	0.04%	0.005%
46	7.201	1914	1916	1919	rVB	1074	515	0.03%	0.004%
47	7.243	1926	1929	1936	rVB3	905	940	0.06%	0.007%
48	7.317	1940	1952	1971	rBV	784669	1370740	83.47%	10.263%
49	7.622	2037	2047	2069	rBV	155276	270337	16.46%	2.024%
50	7.834	2108	2113	2115	rBV3	944	730	0.04%	0.005%
51	7.857	2115	2120	2124	rBV5	2063	2313	0.14%	0.017%
52	7.940	2137	2146	2155	rBV2	4873	7883	0.48%	0.059%
53	8.091	2181	2193	2221	rBV	351024	629817	38.35%	4.715%
54	8.413	2291	2293	2298	rVB4	1180	759	0.05%	0.006%
55	8.445	2301	2303	2305	rBV2	454	300	0.02%	0.002%
56	8.609	2351	2354	2356	rBV2	491	328	0.02%	0.002%
57	8.741	2393	2395	2398	rBV	509	283	0.02%	0.002%
58	8.783	2404	2408	2411	rBV	568	392	0.02%	0.003%
59	8.854	2415	2430	2460	rBV	897250	1478430	90.03%	11.069%
60	9.143	2514	2520	2521	rBV4	1517	1531	0.09%	0.011%
61	9.358	2583	2587	2588	rBV	711	442	0.03%	0.003%
62	9.558	2642	2649	2652	rBV4	1706	1939	0.12%	0.015%
63	9.702	2689	2694	2698	rVB3	645	525	0.03%	0.004%
64	9.735	2698	2704	2705	rBV3	787	738	0.04%	0.006%
65	9.924	2758	2763	2764	rBV2	527	396	0.02%	0.003%
66	9.937	2764	2767	2770	rBV2	993	671	0.04%	0.005%
67	10.034	2794	2797	2800	rVB2	536	357	0.02%	0.003%
68	10.062	2800	2806	2809	rBV	542	594	0.04%	0.004%
69	10.130	2821	2827	2834	rVB5	2694	3488	0.21%	0.026%
70	10.220	2843	2855	2875	rBV	546436	863379	52.58%	6.464%
71	10.316	2883	2885	2890	rVB3	822	420	0.03%	0.003%
72	10.384	2898	2906	2918	rVB4	5508	9474	0.58%	0.071%
73	10.548	2951	2957	2962	rBV5	1382	1689	0.10%	0.013%
74	10.625	2979	2981	2985	rVB2	636	359	0.02%	0.003%
75	10.667	2989	2994	2996	rBV	490	375	0.02%	0.003%
76	10.773	3025	3027	3031	rVB	518	344	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
 Data File : VV021039.D
 Acq On : 16 Apr 2021 11:41
 Operator : SY/MD
 Sample : M2031-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG541

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
 Title : VOC Analysis

77	10.802	3031	3036	3039	rBV2	292	300	0.02%	0.002%
78	10.860	3050	3054	3058	rBV2	809	754	0.05%	0.006%
79	10.924	3064	3074	3082	rBV8	3292	5143	0.31%	0.039%
80	11.008	3095	3100	3104	rVB	317	301	0.02%	0.002%
81	11.136	3136	3140	3141	rBV3	945	628	0.04%	0.005%
82	11.255	3165	3177	3196	rBV	926686	1437014	87.51%	10.759%
83	11.509	3252	3256	3258	rVV2	1437	1179	0.07%	0.009%
84	11.542	3259	3266	3279	rVV5	8840	15110	0.92%	0.113%
85	11.628	3282	3293	3315	rVV	900222	1397268	85.09%	10.461%
86	11.959	3393	3396	3401	rVB3	611	484	0.03%	0.004%
87	12.001	3407	3409	3416	rVV3	553	572	0.03%	0.004%
88	12.046	3420	3423	3425	rBV2	636	369	0.02%	0.003%
89	12.104	3436	3441	3444	rBV	666	608	0.04%	0.005%
90	12.175	3459	3463	3467	rBV	729	467	0.03%	0.003%
91	12.252	3484	3487	3489	rBV	1103	711	0.04%	0.005%
92	12.358	3516	3520	3526	rVB5	1857	1867	0.11%	0.014%
93	12.548	3574	3579	3581	rBV	508	387	0.02%	0.003%
94	12.648	3604	3610	3611	rBV3	1169	846	0.05%	0.006%
95	12.860	3671	3676	3678	rBV2	462	369	0.02%	0.003%
96	13.104	3746	3752	3753	rBV3	636	598	0.04%	0.004%
97	13.156	3763	3768	3770	rBV2	700	592	0.04%	0.004%
98	13.271	3797	3804	3807	rBV6	1317	1728	0.11%	0.013%
99	13.808	3969	3971	3975	rBV3	799	487	0.03%	0.004%
100	14.278	4115	4117	4119	rBV	600	339	0.02%	0.003%




Sum of corrected areas: 13356382

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021039.D
Acq On : 16 Apr 2021 11:41
Operator : SY/MD
Sample : M2031-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG541

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

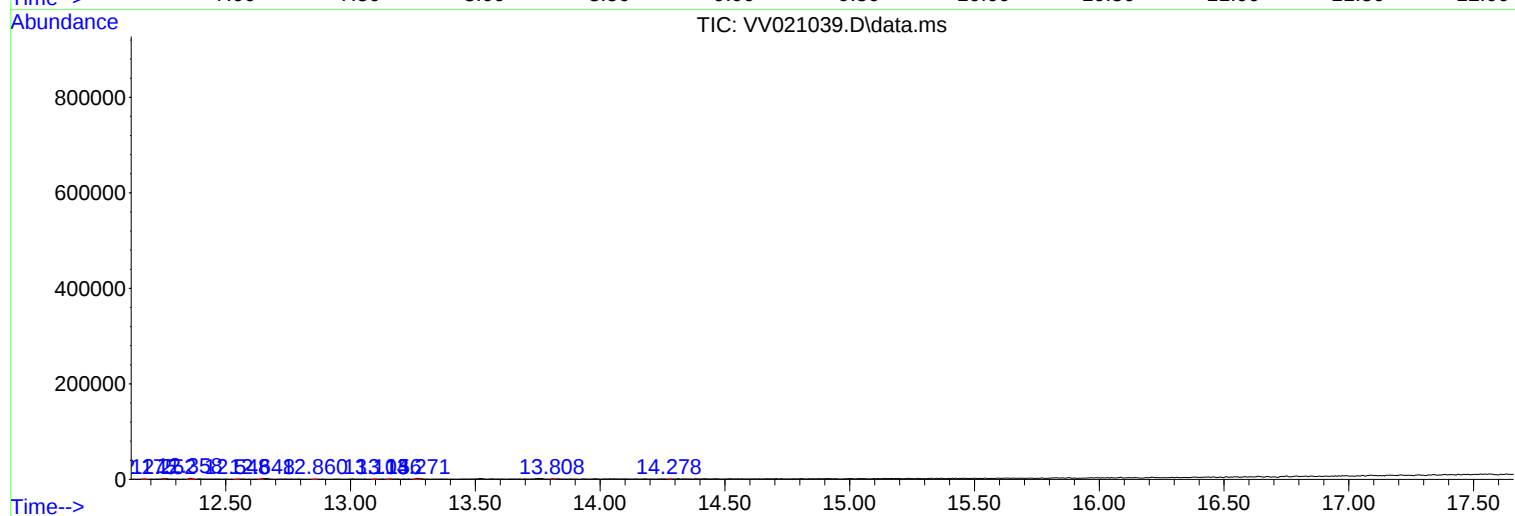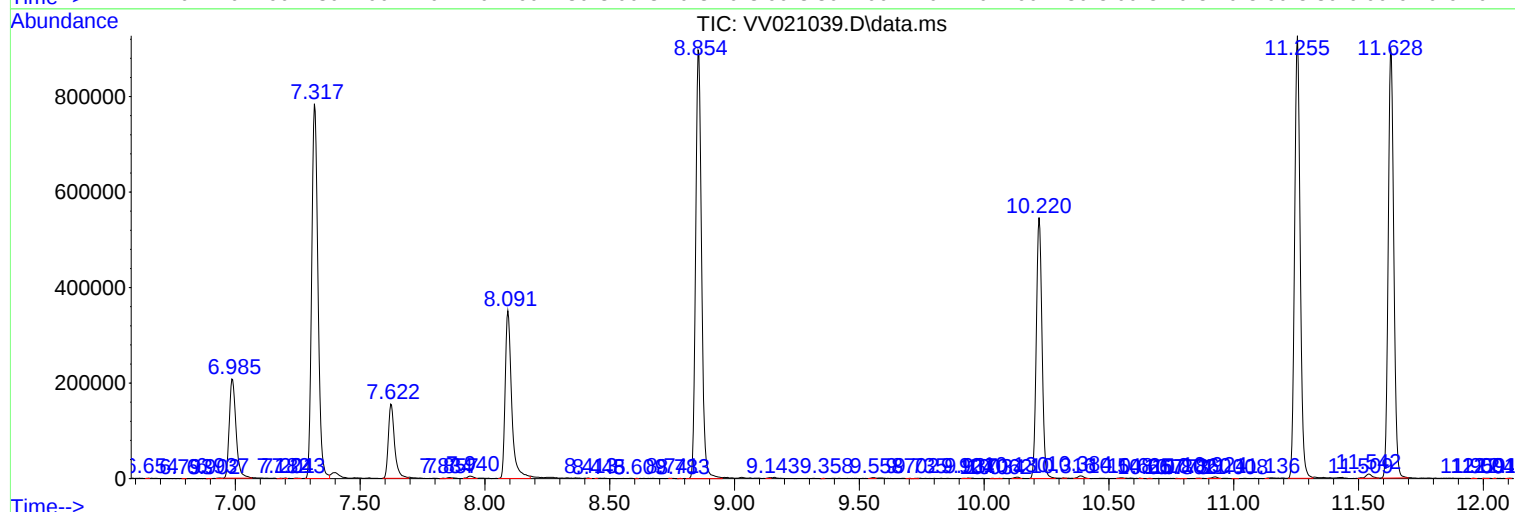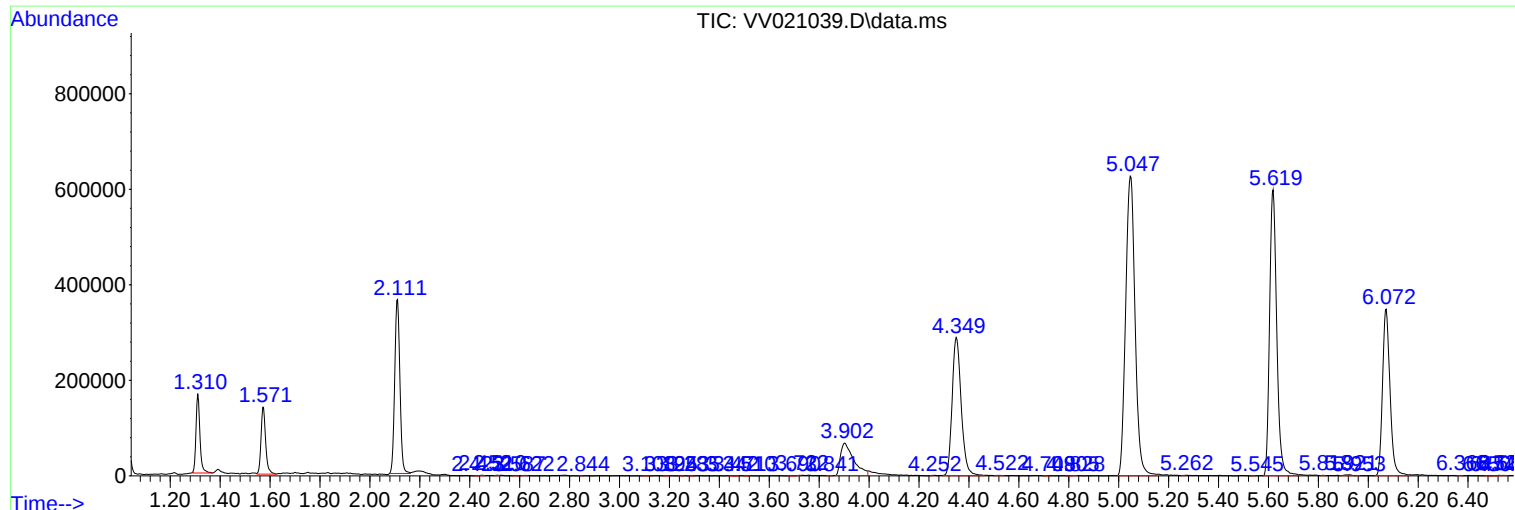

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021039.D
Acq On : 16 Apr 2021 11:41
Operator : SY/MD
Sample : M2031-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG541

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041621\
Data File : VV021039.D
Acq On : 16 Apr 2021 11:41
Operator : SY/MD
Sample : M2031-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG541

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041421WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
